

Alcotest 7110 Calibration Record


Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0037
Location: WALL TOWNSHIP POLICE
Calibration File No.: 00346 Calib. Date: 09/29/2010 Calib. No.: 00010
Certification File No.: 00266 Cert. Date: 05/03/2010 Cert. No.: 00005
Linearity File No.: 00267 Lin. Date: 05/03/2010 Lin. No.: 00005
Solution File No.: 00345 Soln. Date: 09/29/2010 Soln. No.: 00059
Sequential File No.: 00346 File Date: 09/29/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0015
Control Solution %: 0.100% Expires: 04/22/2011
Solution Control Lot: 09D065 Bottle No.: 0295

Coordinator

Last Name: SNYDER First Name: THOMAS MI: J.
Signature: TPR. I Thomas J. Snyder # 5792 Badge No.: 5792
Date: 09/29/2010

*Black Key Temperature Probe Serial.....# DDXKP2-416 JS
*Digital NIST Temperature Measuring System Serial.....# 101 685 673 JS

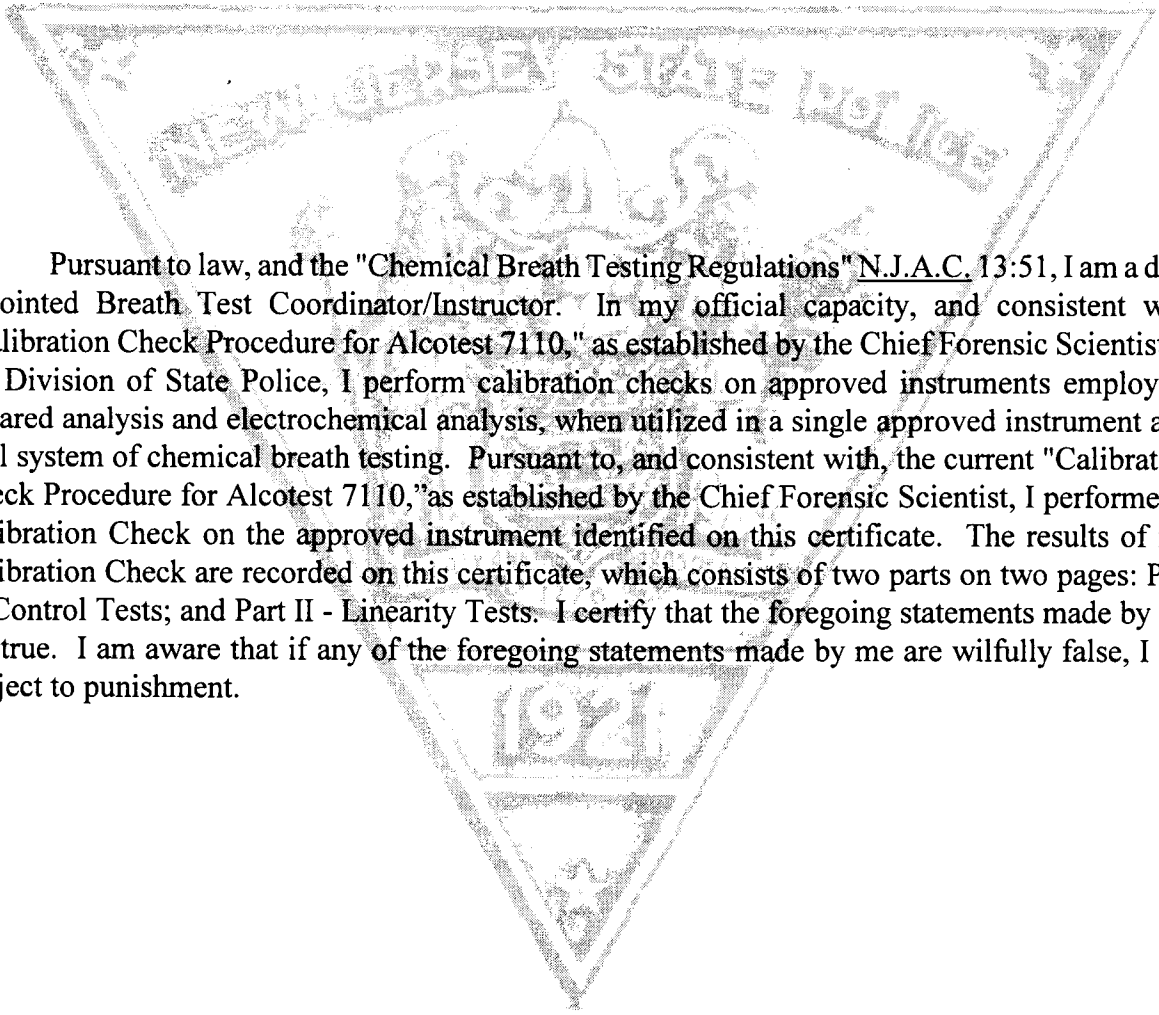

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: WALL TOWNSHIP POLICE
Serial No.: ARXA-0037
Calibration File No.: 00346 Calib. Date: 09/29/2010 Calib. No.: 00010
Certification File No.: 00347 Cert. Date: 09/29/2010 Cert. No.: 00006
Linearity File No.: 00267 Lin. Date: 05/03/2010 Lin. No.: 00005
Solution File No.: 00345 Soln. Date: 09/29/2010 Soln. No.: 00059
Sequential File No.: 00347 File Date: 09/29/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0015
Control Solution %: 0.100% Expires: 04/22/2011
Solution Control Lot: 09D065 Bottle No.: 0295

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	08:49D		
Control 1 EC	0.099%	08:49D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	08:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:50D		
Control 2 EC	0.099%	08:51D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	08:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:51D		
Control 3 EC	0.098%	08:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	08:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	08:53D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: THOMAS J. SNYDER #5792

Badge No.: 5792

Date: 09/29/2010

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0037
Location: WALL TOWNSHIP POLICE
Calibration File No.: 00346 Calib. Date: 09/29/2010 Calib. No.: 00010
Certification File No.: 00347 Cert. Date: 09/29/2010 Cert. No.: 00006
Linearity File No.: 00348 Lin. Date: 09/29/2010 Lin. No.: 00006
Solution File No.: 00345 Soln. Date: 09/29/2010 Soln. No.: 00059
Sequential File No.: 00348 File Date: 09/29/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0003
Control Solution %: 0.040% Expires: 01/12/2012
Solution Control Lot: 10A073 Bottle No.: 0379

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0184
Control Solution %: 0.080% Expires: 01/15/2012
Solution Control Lot: 10A074 Bottle No.: 0379

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0009
Control Solution %: 0.160% Expires: 01/21/2012
Solution Control Lot: 10A075 Bottle No.: 0379

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	09:09D		
Control 1 EC	0.041%	09:09D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	09:09D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:11D		
Control 2 EC	0.040%	09:11D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	09:11D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:13D		
Control 3 EC	0.082%	09:13D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.080%	09:13D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15D		
Control 4 EC	0.080%	09:16D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.080%	09:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:17D		
Control 5 EC	0.162%	09:18D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.161%	09:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19D		
Control 6 EC	0.158%	09:20D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.161%	09:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:22D		

All tests within acceptable tolerance.

Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder # 5792

Badge No.: 5792

Date: 09/29/2010

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0037
Location: WALL TOWNSHIP POLICE
Calibration File No.: 00346 Calib. Date: 09/29/2010 Calib. No.: 00010
Certification File No.: 00347 Cert. Date: 09/29/2010 Cert. No.: 00006
Linearity File No.: 00348 Lin. Date: 09/29/2010 Lin. No.: 00006
Solution File No.: 00349 Soln. Date: 09/29/2010 Soln. No.: 00060
Sequential File No.: 00349 File Date: 09/29/2010

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0015
Control Solution %: 0.100% Expires: 12/31/2011
Solution Control Lot: 09L072 Bottle No.: 1157

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	10:33D		
Control 1 EC	0.102%	10:33D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:34D		
Control 2 EC	0.100%	10:35D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:35D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35D		
Control 3 EC	0.100%	10:36D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:36D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:37D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDXK P2-393

(Signature)

Changed By:

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: *TPR. I Thomas J. Snyder #5792*

Badge No.: 5792

Date: 09/29/2010



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDRKS3-0003

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXDS3-0184

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDSCS3-0009

Certification Date

Technician

Re-Certification Due Date

2/3/10

DM

2/3/11

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXKP3-416

2/5/10

2/5/11

Probe Value

102

Dräger Safety Diagnostics, Inc.
Technical Service Department

DM



Calibration
Certificate No. 1750.01

**Calibration complies with ISO 9001
ISO/IEC 17025 AND ANSI/NCSL Z540-1**



Cert. No.: 4000-2924450

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, P.O. Box 2158, Secaucus, NJ 07094 U.S.A.

Instrument Identification:

Model: 61220-601 S/N: 101685673 Manufacturer : Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	11/19/10	A9B21010
Temperature Probe	128	12/10/10	A9B23079
Temperature Calibration Bath TC-231	A79341		
Temperature Probe	3039	12/10/10	A9B23080-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Module	A27129	7/09/10	1000264338
Temperature Probe	5202	3/11/11	B0310050
Temperature Calibration Bath TC-256	B01375		
Temperature Probe	157	7/27/10	A9708011-4

Certificate Information:

Technician: 68 Procedure: CAL-06 Cal Date: 5/17/10 Cal Due: 5/17/12
 Test Conditions: 23.5°C 47.0 %RH 1017 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±uc	TUR
°C		N.A.		0.002	-0.001	Y	-0.048	0.052	0.013	3.8:1
°C		N.A.		25.001	25.000	Y	24.951	25.051	0.013	3.8:1
°C		N.A.		60.002	60.000	Y	59.952	60.052	0.018	2.8:1
°C		N.A.		100.000	99.999	Y	99.950	100.050	0.013	3.8:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±uc=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = Nominal(Rounded) - Tolerance; Max = Nominal(Rounded) + Tolerance; Date=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Wallace Berry
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
 Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
 International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 7/7/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10F079

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1183 to 0.1190 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 10, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek, M.S.
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 20th day of July, 2010.
Handwritten signature of Linda L. Desantis
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 1/19/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10L084

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1185 to 0.1190 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 16, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 24th day of January, 2011.

Linda L. Desantis
 Notary

Linda L. Desantis
 Notary Public, New Jersey
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

JON S. CORZINE
Governor

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 5/08/2009

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 09D065

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1201 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 22, 2011.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Handwritten signature of Ajit R. Tungare]

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of May, 2009.

[Handwritten signature of Linda L. DeSantis]
Notary

Linda L. DeSantis
My Commission
Expires Aug. 17, 2009





CHRIS CHRISTIE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

PAULA T. DOW
Acting Attorney General
COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 2/2/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A073

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0479 to 0.0481 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 12, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Kenneth W. Klawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.

Notary

Linda L. Decaris
Notary Public, New Jersey
Commission Expires 6-17-14



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

PAULA T. DOW
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 2/3/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A074

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0954 to 0.0958 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 15, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

[Signature]
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.

[Signature]
Notary

Linda L. Desantis
Notary Public, New Jersey
My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

PAULA T. DOW
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.


ANALYSIS DATE: 2/4/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10A075


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1913 to 0.1919 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is January 21, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


 Kenneth W. Kawalek, M.S.
 Assistant Chief Forensic Scientist
 Division of State Police

Sworn to and subscribed before me this 19th day of February, 2010.


 Notary

Linda L. Decaria
 Notary Public, New Jersey
 My Commission Expires 6-17-14



New Jersey Is An Equal Opportunity Employer





CHRIS CHRISTIE
Governor

State of New Jersey
OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

PAULA T. DOW
Acting Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 1/15/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 09L072

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1203 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 31, 2011.

As the Director of Office of Forensic Sciences, Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Howard J. Baum, Ph.D.
Director, Office of Forensic Sciences
Division of State Police

Sworn to and subscribed before me this 21 day of January, 2010.

Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Law and Public Safety
This is to certify that

Thomas J. Snyder
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF February
TWO THOUSAND AND SIX

Joseph P. Rinaldi
SUPERINTENDENT
NEW JERSEY STATE POLICE

Zachary V. Zuckerman
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 03/27/08	SUSSEX F.A.	TY. RULL
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 01/06)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Thomas J. Snyder
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF
THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C
A METHOD TO DETERMINE INTOXICATION.
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 17th DAY OF June
TWO THOUSAND AND SIX

Joseph P. Rinaldi
SUPERINTENDENT
NEW JERSEY STATE POLICE

Zachary V. Zuckerman
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 03/27/08	SUSSEX F.A.	TY. RULL
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 01/06)

DEPARTMENT OF
Law and Public Safety
This is to certify that

Thomas J. Snyder
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER
142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breathalyzer TO DETERMINE
INTOXICATION
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 11th DAY OF Aug.
TWO THOUSAND AND 00

Kevin P. Rinaldi
SUPERINTENDENT
NEW JERSEY STATE POLICE

Zachary V. Zuckerman
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. 11-14-04	ALTC	Phil Lanzetta
2. 5-5-03	OCPPA	Phil Lanzetta
3. 4-4-05	ACTC	C. V. ...
4. 7-26-07	OLPA	B. ...
5.		
6.		
7.		
8.		
9.		

SP-293B (Rev. 11/99)

Drägersafety

Alcotest[®] 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

SERIAL NUMBER:

11-20-2008

ARXA-0037

Draeger Safety Diagnostics, Inc.

A handwritten signature in black ink, appearing to be 'J. K.', is written over a horizontal line.



Drägersafety

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDAB-0015

Certification Date

Technician

Re-Certification Due Date

5-26-10

977M

5-26-11

Dräger

safety

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXKP2-393

5-26-10

5-26-11

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

977M