

# Alcotest 7110 Calibration Record


## Equipment

|                                |                         |                         |
|--------------------------------|-------------------------|-------------------------|
| Alcotest 7110 MKIII-C          | Serial No.: ARZL-0146   |                         |
| Location: WALL TOWNSHIP POLICE |                         |                         |
| Calibration File No.: 00086    | Calib. Date: 11/12/2009 | Calib. No.: 00005       |
| Certification File No.: 00027  | Cert. Date: 05/19/2009  | Cert. No.: 00002        |
| Linearity File No.: 00028      | Lin. Date: 05/19/2009   | Lin. No.: 00002         |
| Solution File No.: 00083       | Soln. Date: 10/31/2009  | Soln. No.: 00016        |
| Sequential File No.: 00086     | File Date: 11/12/2009   |                         |
| Calibrating Unit: WET          | Model No.: CU-34        | Serial No.: DDXB S3-113 |
| Control Solution %: 0.100%     |                         | Expires: 04/22/2011     |
| Solution Control Lot: 09D065   |                         | Bottle No.: 0499        |

## Coordinator

Last Name: SNYDER First Name: THOMAS MI: J.  
Signature: TH. I. Thomas J. Snyder #5792 Badge No.: 5792  
Date: 11/12/2009

- \*Black Key Temperature Probe Serial.....# DDUN P2-229 JJS
- \*Digital NIST Temperature Measuring System Serial.....# 806 375 77 JJS

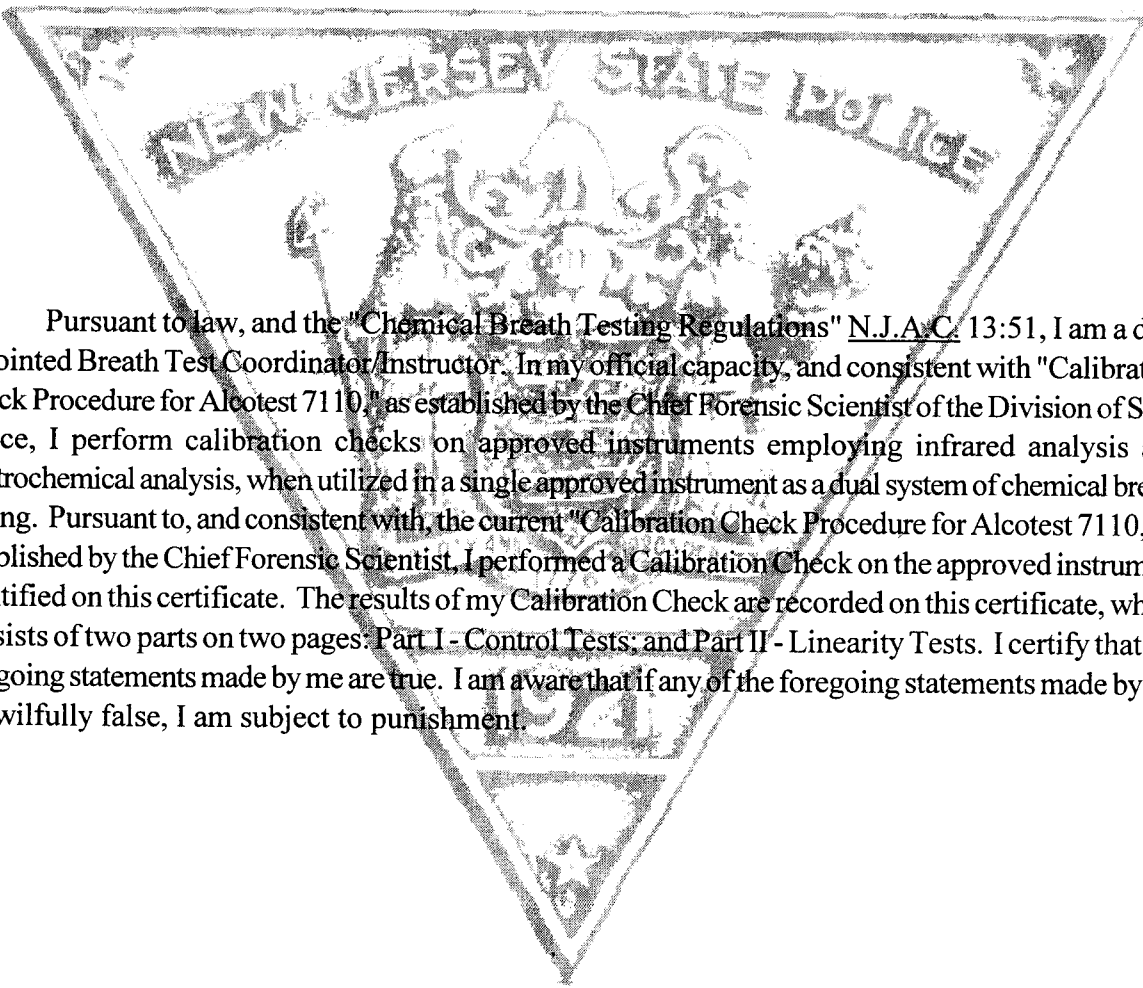

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARZL-0146  
Location: WALL TOWNSHIP POLICE  
Calibration File No.: 00086 Calib. Date: 11/12/2009 Calib. No.: 00005  
Certification File No.: 00087 Cert. Date: 11/12/2009 Cert. No.: 00003  
Linearity File No.: 00028 Lin. Date: 05/19/2009 Lin. No.: 00002  
Solution File No.: 00083 Soln. Date: 10/31/2009 Soln. No.: 00016  
Sequential File No.: 00087 File Date: 11/12/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXB S3-113  
Control Solution %: 0.100% Expires: 04/22/2011  
Solution Control Lot: 09D065 Bottle No.: 0499

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 14:16S |                |                     |
| Control 1 EC      | 0.099% | 14:17S | 33.9°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.101% | 14:17S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:17S |                |                     |
| Control 2 EC      | 0.098% | 14:18S | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.099% | 14:18S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:19S |                |                     |
| Control 3 EC      | 0.099% | 14:20S | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.101% | 14:20S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:20S |                |                     |

All tests within acceptable tolerance.

### Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 11/12/2009

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARZL-0146  
Location: WALL TOWNSHIP POLICE  
Calibration File No.: 00086 Calib. Date: 11/12/2009 Calib. No.: 00005  
Certification File No.: 00087 Cert. Date: 11/12/2009 Cert. No.: 00003  
Linearity File No.: 00088 Lin. Date: 11/12/2009 Lin. No.: 00003  
Solution File No.: 00083 Soln. Date: 10/31/2009 Soln. No.: 00016  
Sequential File No.: 00088 File Date: 11/12/2009

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRK S3-0003  
Control Solution %: 0.040% Expires: 06/26/2010  
Solution Control Lot: 08F054 Bottle No.: 1087

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXD S3-0184  
Control Solution %: 0.080% Expires: 06/28/2010  
Solution Control Lot: 08F055 Bottle No.: 0087

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDSC S3-0009  
Control Solution %: 0.160% Expires: 07/07/2010  
Solution Control Lot: 08G057 Bottle No.: 0164

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 14:34S |                |                     |
| Control 1 EC      | 0.042% | 14:34S | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.039% | 14:34S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:36S |                |                     |
| Control 2 EC      | 0.041% | 14:37S | 34.0°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.039% | 14:37S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:38S |                |                     |
| Control 3 EC      | 0.081% | 14:39S | 34.0°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.080% | 14:39S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:40S |                |                     |
| Control 4 EC      | 0.081% | 14:41S | 34.0°C         | *** TEST PASSED *** |
| Control 4 IR      | 0.081% | 14:41S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:43S |                |                     |
| Control 5 EC      | 0.161% | 14:43S | 33.9°C         | *** TEST PASSED *** |
| Control 5 IR      | 0.162% | 14:43S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:45S |                |                     |
| Control 6 EC      | 0.159% | 14:46S | 33.9°C         | *** TEST PASSED *** |
| Control 6 IR      | 0.162% | 14:46S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 14:47S |                |                     |

All tests within acceptable tolerance.

### Coordinator

Last Name: SNYDER

First Name: THOMAS

MI: J.

Signature: TPR. I Thomas J. Snyder #5792

Badge No.: 5792

Date: 11/12/2009

# Calibrating Unit

## New Standard Solution Report

|                         |                       |              |             |
|-------------------------|-----------------------|--------------|-------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C | Serial No.:  | ARZL-0146   |
| Location:               | WALL TOWNSHIP POLICE  |              |             |
| Calibration File No.:   | 00086                 | Calib. Date: | 11/12/2009  |
| Certification File No.: | 00087                 | Cert. Date:  | 11/12/2009  |
| Linearity File No.:     | 00088                 | Lin. Date:   | 11/12/2009  |
| Solution File No.:      | 00089                 | Soln. Date:  | 11/12/2009  |
| Sequential File No.:    | 00089                 | File Date:   | 11/12/2009  |
|                         |                       | Calib. No.:  | 00005       |
|                         |                       | Cert. No.:   | 00003       |
|                         |                       | Lin. No.:    | 00003       |
|                         |                       | Soln. No.:   | 00017       |
| <br>                    |                       |              |             |
| Calibrating Unit:       | WET                   | Model No.:   | CU-34       |
| Control Solution %:     | 0.100%                | Serial No.:  | DDXB S3-113 |
| Solution Control Lot:   | 08L061                | Expires:     | 12/01/2010  |
|                         |                       | Bottle No.:  | 0790        |

| Function          | Result | Time   | Temperature    | Comment(s)          |
|-------------------|--------|--------|----------------|---------------------|
|                   | %BAC   | HH:MM  | Simulator (°C) | or Error(s)         |
| Ambient Air Blank | 0.000% | 15:56S |                |                     |
| Control 1 EC      | 0.102% | 15:56S | 34.0°C         | *** TEST PASSED *** |
| Control 1 IR      | 0.102% | 15:56S | 34.0°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:57S |                |                     |
| Control 2 EC      | 0.101% | 15:58S | 33.9°C         | *** TEST PASSED *** |
| Control 2 IR      | 0.101% | 15:58S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 15:58S |                |                     |
| Control 3 EC      | 0.101% | 15:59S | 33.9°C         | *** TEST PASSED *** |
| Control 3 IR      | 0.101% | 15:59S | 33.9°C         | *** TEST PASSED *** |
| Ambient Air Blank | 0.000% | 16:00S |                |                     |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL NUMBER: DDWS P2-284 

**Changed By:**

|   |                    |                  |
|---|--------------------|------------------|
| Last Name: SNYDER                               | First Name: THOMAS | MI: J.           |
| Signature: <u>TPR. I Thomas J. Snyder #5792</u> |                    | Badge No.: 5792  |
|   |                    | Date: 11/12/2009 |



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDK53-1003

Certification Date

Technician

Re-Certification Due Date

02/03/2009

[Signature]

02/03/2010



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDK53-0184

Certification Date

Technician

Re-Certification Due Date

02/03/2009

[Signature]

02/03/2010



Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDSC 53.0009

Certification Date

Technician

Re-Certification Due Date

02-03-09

[Signature]

02-03-10

## Drägersafety

### ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDUNP2-229

02/03/2009

02/03/2010

Probe Value

103

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

[Signature]



Calibration  
Certificate No. 1750.01

**Calibration complies with ISO 9001  
ISO/IEC 17025 AND ANSI/NCSL Z540-1**



**Cert. No.: 4000-2035919**

**Traceable® Certificate of Calibration for Digital Thermometer**

**Instrument Identification:**

Model: 61220-601      S/N: 80637577      Manufacturer : Control Company

**Standards/Equipment:**

| Description   | Serial Number | Due Date | NIST Traceable Reference |
|---|---------------|----------|--------------------------|
| Temperature Probe<br>Thermistor Module                  | 149           | 3/06/09  | A82225037-3              |
| Temperature Calibration Bath TC218<br>Thermistor Module | A27129        | 8/22/09  | 1000248949               |
| Temperature Calibration Bath TC155<br>Thermistor Module | A73332        |          |                          |
| Temperature Calibration Bath TC155<br>Thermistor Module | 93139         |          |                          |
| Temperature Calibration Bath TC155<br>Thermistor Module | A27129        | 8/22/09  | 1000248949               |
| Temperature Calibration Bath TC155<br>Temperature Probe | 157           | 5/28/09  | A8519038-4               |

**Certificate Information:**

Technician: 68      Procedure: CAL-06      Cal Date: 11/18/08      Cal Due: 11/18/10  
Test Conditions: 25.0°C      34.0 %RH      1031 mBar

**Calibration Data: (New Instrument)**

| Unit(s) | Nominal | As Found | In Tol | Nominal | As Left | In Tol | Min    | Max     | ±uc   | TUR   |
|---------|---------|----------|--------|---------|---------|--------|--------|---------|-------|-------|
| °C      |         | N.A.     |        | 0.001   | 0.000   | Y      | -0.049 | 0.051   | 0.013 | 3.8:1 |
| °C      |         | N.A.     |        | 25.001  | 24.998  | Y      | 24.951 | 25.051  | 0.013 | 3.8:1 |
| °C      |         | N.A.     |        | 60.001  | 60.000  | Y      | 59.951 | 60.051  | 0.018 | 2.8:1 |
| °C      |         | N.A.     |        | 100.001 | 99.997  | Y      | 99.951 | 100.051 | 0.013 | 3.8:1 |

**This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.**

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±uc=Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Date=MM/DD/YY

*Wallace Berry*  
Wallace Berry, Technical Manager

**Maintaining Accuracy:**

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

**Recalibration:**

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

**CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA**  
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2000 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-AQ-HOU.  
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

JON S. CORZINE  
 Governor

ANNE MILGRAM  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 5/08/2009

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 09D065

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1201 to 0.1210 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 22, 2011.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
 Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 19<sup>th</sup> day of May, 2009.

Notary



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable







JON S. CORZINE  
Governor

State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

ANNE MILGRAM  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

**MANUFACTURER: Drager Safety, Inc.      ANALYSIS DATE: 07/16/2008**

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F054**

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0487 to 0.0493 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 26, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 19<sup>th</sup> day of August, 2008.

Notary  
JOHN R. LEAVER  
NOTARY PUBLIC STATE OF NEW JERSEY  
MY COMMISSION EXPIRES 12/14/2012



New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/25/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08F055

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.0977 to 0.0984 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 28, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare (Handwritten signature)

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

Notary (Handwritten signature)

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

JON S. CORZINE
Governor

ANNE MILGRAM
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc. ANALYSIS DATE: 07/28/2008

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 08G057

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1956 to 0.1959 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 7, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare (Handwritten signature)

Ajit R. Tungare
Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 19th day of August, 2008.

(Handwritten signature of John R. Leaver)
Notary

JOHN R. LEAVER
NOTARY PUBLIC STATE OF NEW JERSEY
MY COMMISSION EXPIRES 12/14/2012





JON S. CORZINE  
Governor

State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

ANNE MILGRAM  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

**MANUFACTURER:** Drager Safety, Inc.      **ANALYSIS DATE:** 12/23/2008

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 08L061

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have an ethyl alcohol concentration range of 0.1201 to 0.1206 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 1, 2010.

As Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ajit R. Tungare  
Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 14<sup>th</sup> day of January, 2009.

Linda L. DeSantis  
Notary

**Linda L. DeSantis**  
**My Commission**  
**Expires Aug. 17, 2009**



New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable



DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Thomas J. Snyder**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE ALCOTEST 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 22nd DAY OF February TWO THOUSAND AND SIX

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

|    | DATE     | Refresher Course PLACE | INSTRUCTOR |
|----|----------|------------------------|------------|
| 1. | 03/27/08 | SUSSEX F.A.            | M. Rull    |
| 2. |          |                        |            |
| 3. |          |                        |            |
| 4. |          |                        |            |
| 5. |          |                        |            |
| 6. |          |                        |            |
| 7. |          |                        |            |
| 8. |          |                        |            |
| 9. |          |                        |            |

S.P. 2938 (Rev. 01/06)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Thomas J. Snyder**  
Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Alcotest 7110 MKIII-C A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 17th DAY OF June TWO THOUSAND AND SIX

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

|    | DATE     | Refresher Course PLACE | INSTRUCTOR |
|----|----------|------------------------|------------|
| 1. | 03/27/08 | SUSSEX F.A.            | M. Rull    |
| 2. |          |                        |            |
| 3. |          |                        |            |
| 4. |          |                        |            |
| 5. |          |                        |            |
| 6. |          |                        |            |
| 7. |          |                        |            |
| 8. |          |                        |            |
| 9. |          |                        |            |

S.P. 2938 (Rev. 01/06)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Thomas J. Snyder**  
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1966 IN THE OPERATION OF THE Breathalyzer A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 11th DAY OF Aug. TWO THOUSAND AND 00

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

|    | DATE     | Refresher Course PLACE | INSTRUCTOR        |
|----|----------|------------------------|-------------------|
| 1. | 11-14-01 | ALTC                   | Rick Ferguson     |
| 2. | 5-5-03   | DCPA                   | [Signature]       |
| 3. | 4-4-05   | ACTC                   | C. V. [Signature] |
| 4. | 7-26-07  | OLPA                   | A. [Signature]    |
| 5. |          |                        |                   |
| 6. |          |                        |                   |
| 7. |          |                        |                   |
| 8. |          |                        |                   |
| 9. |          |                        |                   |

SP-2938 (Rev. 11/99)

**Dräger**safety

**Alcotest<sup>®</sup> 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

02-18-2009

SERIAL NUMBER:

AKZL-0146

**Draeger Safety Diagnostics, Inc.**





Drägersafety

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXBS3-113

Certification Date

9-30-09

Technician

mm

Re-Certification Due Date

9-30-10

Drägersafety

ALCOTEST® 7110 TEMPERATURE PROBE

# CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWJP2-284

Certification date:

9-30-09

Next Certification due:

9-30-10

Probe Value

101

Draeger Safety Diagnostics, Inc.  
Technical Service Department

mm