


# Alcotest 7110 Calibration Record

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARZL-0146  
Location: WALL TOWNSHIP POLICE  
Calibration File No.: 00527 Calib. Date: 09/04/2012 Calib. No.: 00011  
Certification File No.: 00460 Cert. Date: 03/07/2012 Cert. No.: 00008  
Linearity File No.: 00461 Lin. Date: 03/07/2012 Lin. No.: 00008  
Solution File No.: 00522 Soln. Date: 08/26/2012 Soln. No.: 00094  
Sequential File No.: 00527 File Date: 09/04/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0015  
Control Solution %: 0.100% Expires: 09/09/2012  
Solution Control Lot: 101082 Bottle No.: 0243

**Coordinator**  
Last Name: DENNIS First Name: MARC MI: W.  
Signature: *Tpr. I J Dennis #5925* Badge No.: 5925  
Date: 09/04/2012

\*Black Key Temperature Probe Serial .....# DDXK P2-323 (10)  
\*Digital NIST Thermometer Serial.....# 122172162 (10)

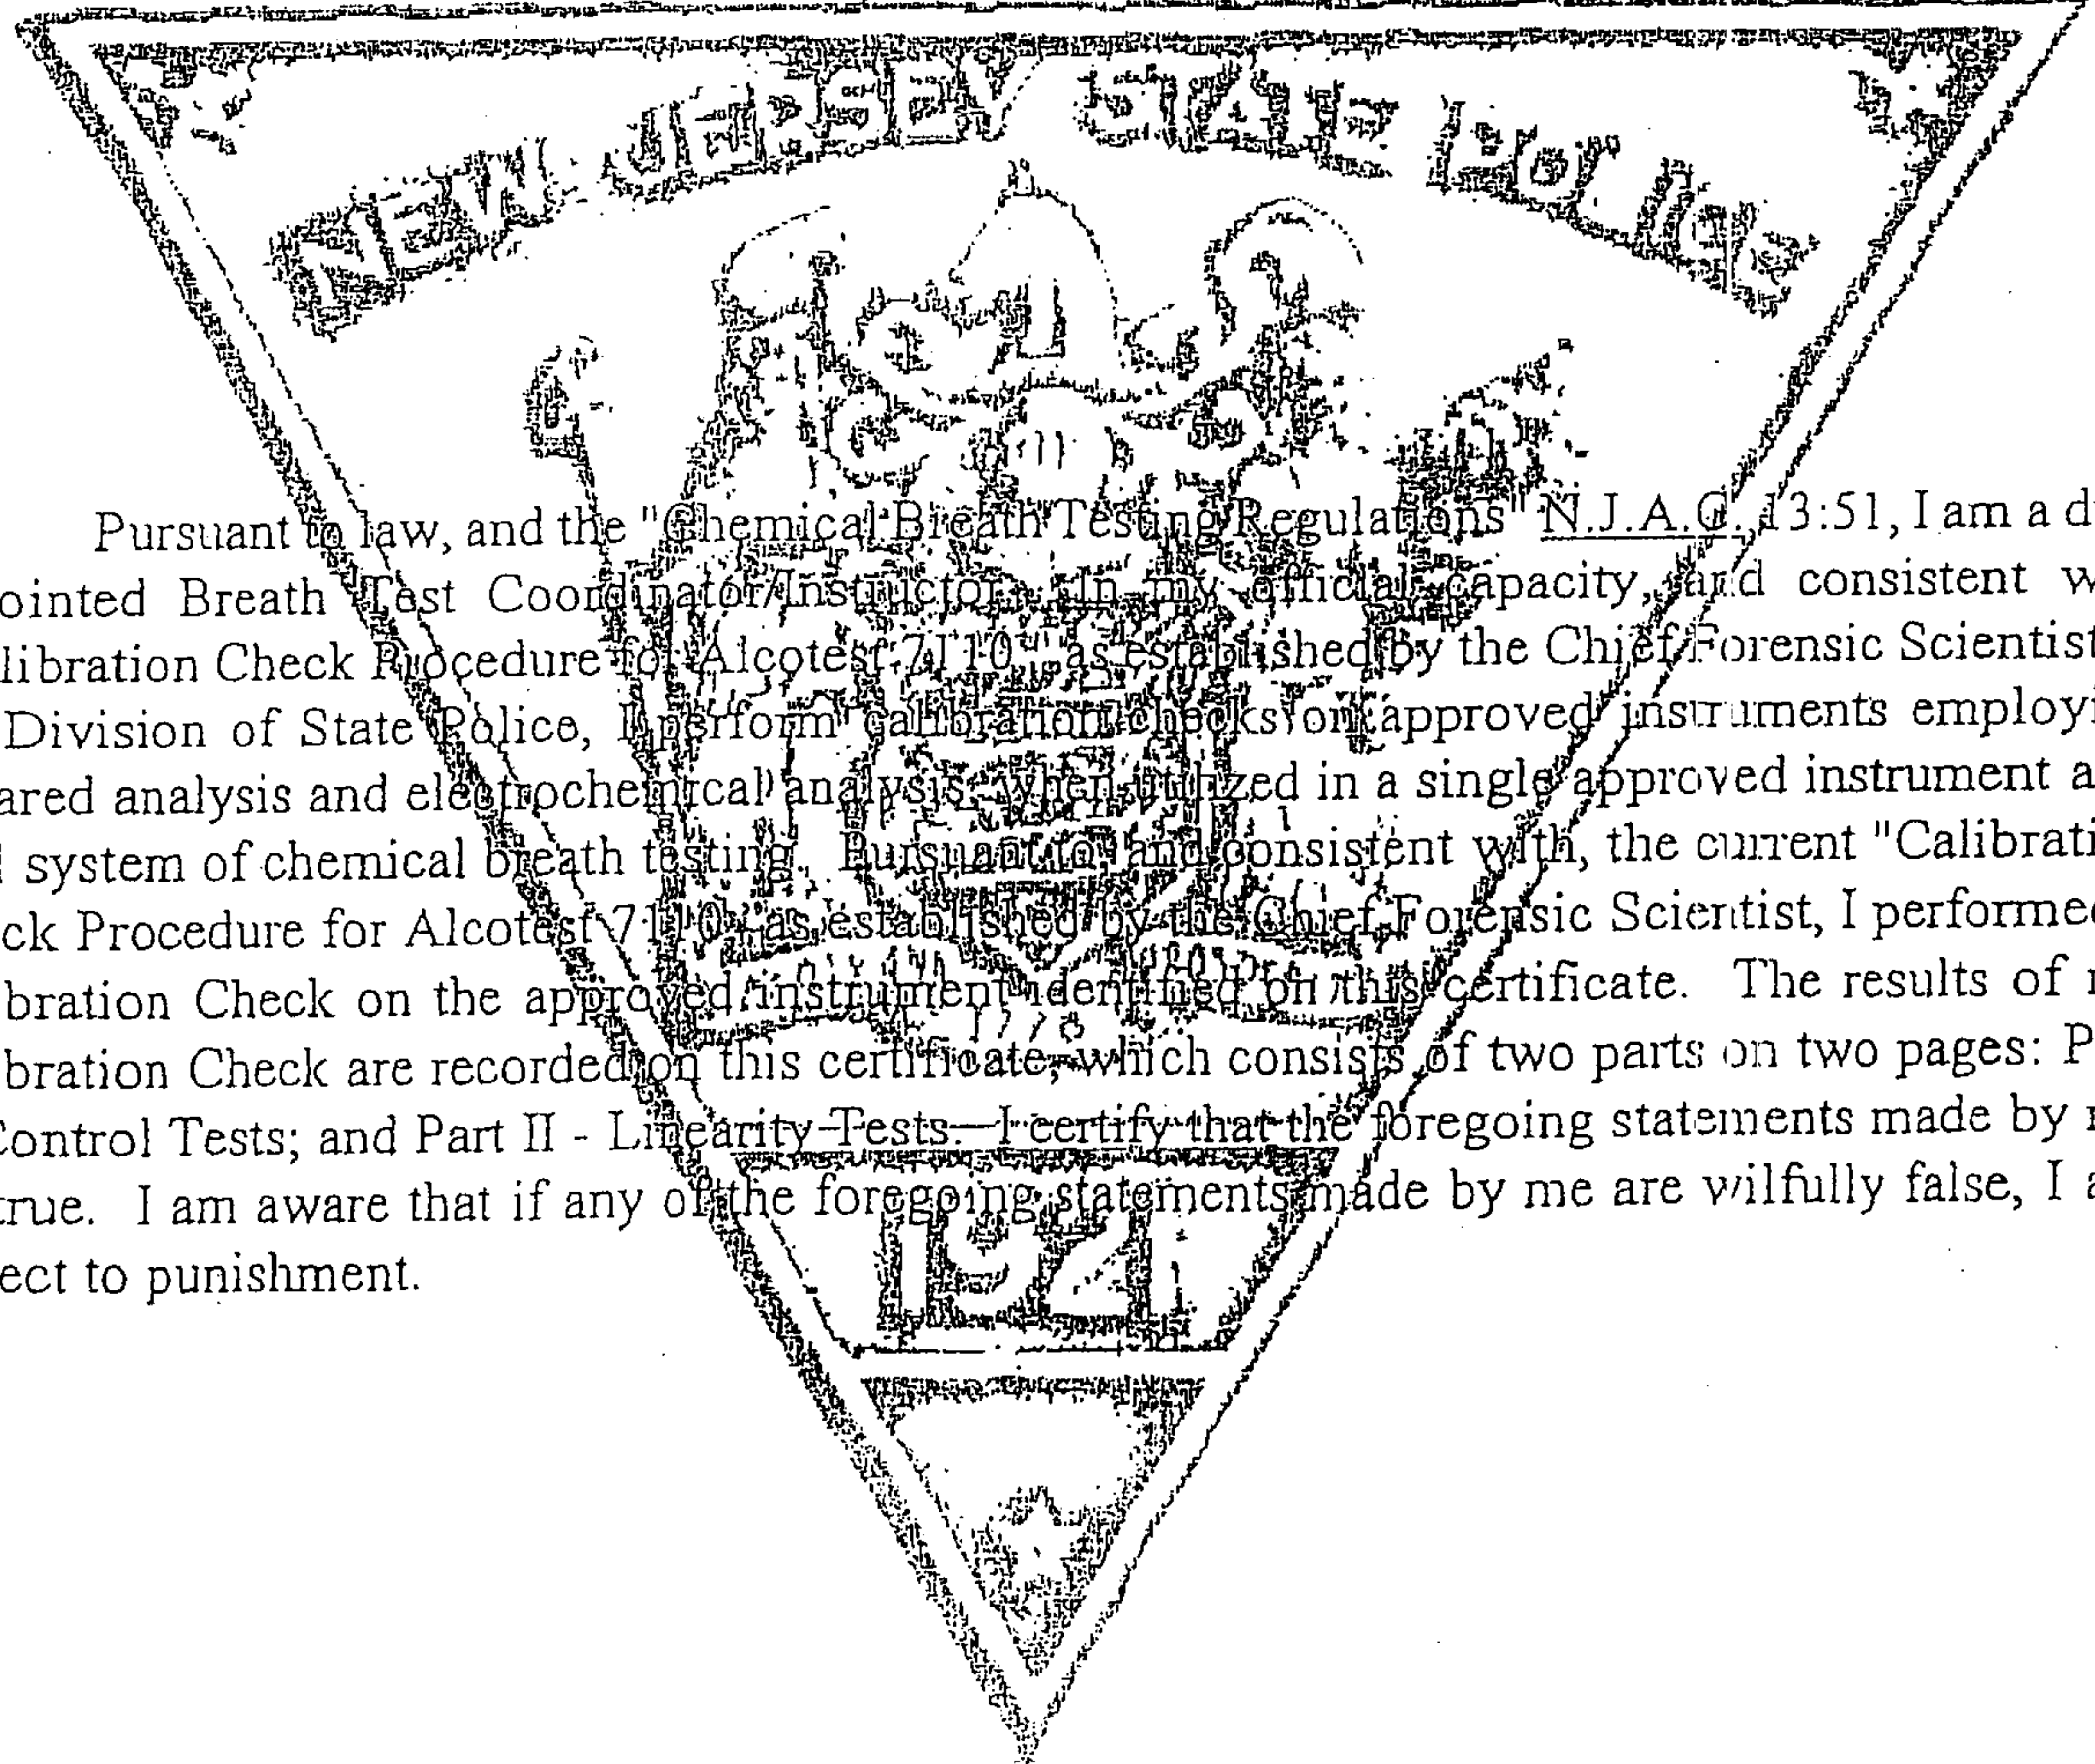

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis. When utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

**Equipment** Alcotest 7110 MKIII-C Serial No.: ARZL-0146  
Location: WALL TOWNSHIP POLICE  
Calibration File No.: 00527 Calib. Date: 09/04/2012 Calib. No.: 00011  
Certification File No.: 00528 Cert. Date: 09/04/2012 Cert. No.: 00009  
Linearity File No.: 00461 Lin. Date: 03/07/2012 Lin. No.: 00008  
Solution File No.: 00522 Soln. Date: 08/26/2012 Soln. No.: 00094  
Sequential File No.: 00528 File Date: 09/04/2012

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0015  
Control Solution %: 0.100% Expires: 09/09/2012  
Solution Control Lot: 10I082 Bottle No.: 0243

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:18D		
Control 1 EC	0.098%	13:18D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:19D		
Control 2 EC	0.098%	13:20D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20D		
Control 3 EC	0.099%	13:21D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	13:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:22D		

All tests within acceptable tolerance.

### Coordinator

Last Name: DENNIS

Signature: TAL. DENNIS

First Name: MARG

MI: W.

Badge No.: 5925

Date: 09/04/2012

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.: ARZL-0146
Location:	WALL TOWNSHIP POLICE	
Calibration File No.:	00527	Calib. Date: 09/04/2012
Certification File No.:	00528	Calib. No.: 00011
Linearity File No.:	00529	Cert. Date: 09/04/2012
Solution File No.:	00522	Cert. No.: 00009
Sequential File No.:	00529	Lin. Date: 09/04/2012
		Lin. No.: 00009
		Soln. Date: 08/26/2012
		Soln. No.: 00094
		File Date: 09/04/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.040%	Serial No.: DDXD S3-0186
Solution Control Lot:	11F090	Expires: 06/27/2013
		Bottle No.: 0371
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.080%	Serial No.: DDXD S3-0188
Solution Control Lot:	11F091	Expires: 06/30/2013
		Bottle No.: 0047
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.160%	Serial No.: DDXD S3-0191
Solution Control Lot:	11G092	Expires: 07/03/2013
		Bottle No.: 0222

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:54D		
Control 1 EC	0.040%	13:55D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.039%	13:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:56D		
Control 2 EC	0.040%	13:57D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	13:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:58D		
Control 3 EC	0.080%	13:59D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.079%	13:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:01D		
Control 4 EC	0.080%	14:01D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.079%	14:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:03D		
Control 5 EC	0.158%	14:03D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.159%	14:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05D		
Control 6 EC	0.156%	14:06D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.158%	14:06D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:08D		

All tests within acceptable tolerance.

**Coordinator**

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: \_\_\_\_\_

*TPR. I [Signature] #5925*

Badge No.: 5925

Date: 09/04/2012

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARZL-0146
Location:	WALL TOWNSHIP POLICE		
Calibration File No.:	00527	Calib. Date:	09/04/2012
Certification File No.:	00528	Cert. Date:	09/04/2012
Linearity File No.:	00529	Lin. Date:	09/04/2012
Solution File No.:	00530	Soln. Date:	09/04/2012
Sequential File No.:	00530	File Date:	09/04/2012
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDAB-0015
Solution Control Lot:	11H094	Expires:	08/17/2013
		Bottle No.:	0251

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:14D		
Control 1 EC	0.101%	15:15D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:15D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:15D		
Control 2 EC	0.099%	15:16D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	15:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17D		
Control 3 EC	0.099%	15:18D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	15:18D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

TEMPERATURE PROBE SERIAL # DDXK P2-393 (M)

**Changed By:**

Last Name: DENNIS


First Name: MARC

MI: W.

Signature: T.D. I [Signature] #5925

Badge No.: 5925

Date: 09/04/2012

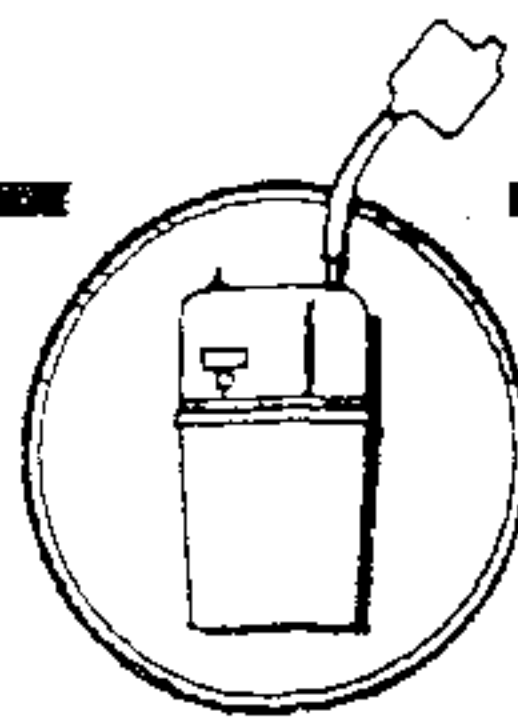

**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXDS3-0186

Certification Date


Technician

Re-Certification Due Date

2/2/12

DM

2/2/13

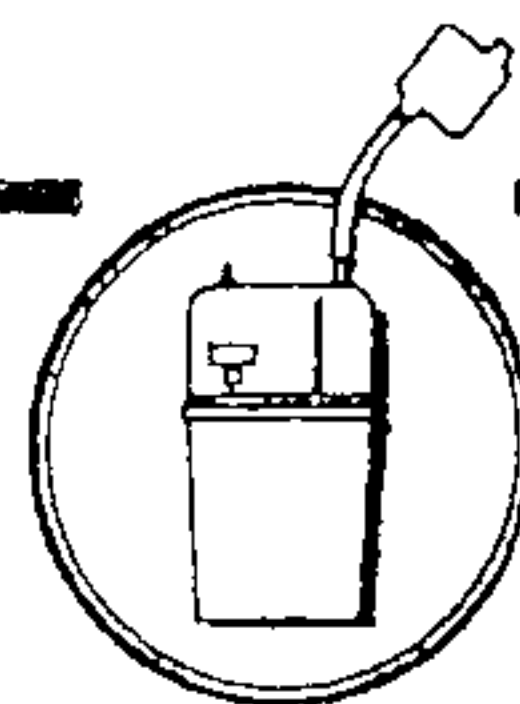

**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDXDS3-0188

Certification Date


Technician

Re-Certification Due Date

2/2/12

DM

2/2/13

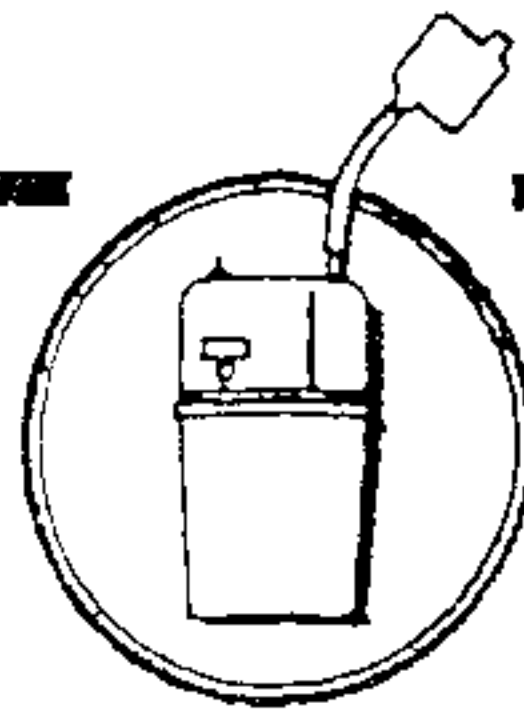

**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

Model: ALCOTEST® CU34

Model: MARK IIA

Other: \_\_\_\_\_

Serial Number:

DDXDS3-0191

Certification Date

Technician

Re-Certification Due Date

2/2/12

DM

2/2/13

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXKP2-323

2/3/12

2/3/13

Probe Value

103

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

DM



Calibration  
Certificate No. 1750.01

Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-4269971

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsenford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601      S/N: 122172162      Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-275	A9A237		
Digital Thermometer	B16815	6/06/12	B1606038
PRT Temperature Probe	01641	5/28/12	B1526085
Temperature Calibration Bath TC-256	B01375		
Thermistor Module	A27129	10/31/12	1000306945
Temperature Probe	157	11/13/12	6-BL72N-1-1
Temperature Calibration Bath TC-179	A45240		
Thermistor Module	A17118	2/01/13	1000311439
Temperature Probe	128	2/14/13	3-BN9WZ-27-1

Certificate Information:

Technician: 68      Procedure: CAL-06      Cal Date: 3/30/12      Cal Due: 3/30/14  
Test Conditions: 23.0°C      44.0 %RH      1012 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		-0.000	-0.002	Y	-0.050	0.050	0.013	3.8:1
°C		N.A.		25.001	24.999	Y	24.951	25.051	0.014	3.6:1
°C		N.A.		60.000	60.000	Y	59.950	60.050	0.018	2.8:1
°C		N.A.		100.001	100.001	Y	99.951	100.051	0.018	2.8:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

*Nicol Rodriguez*  
Nicol Rodriguez, Quality Manager

*Wallace Berry*  
Wallace Berry, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rex Road Friendswood, TX 77546 USA  
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.  
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA)



State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

PAULA T. DOW  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 9/23/2010

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 10I082


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1190 to 0.1194 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 9, 2012.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

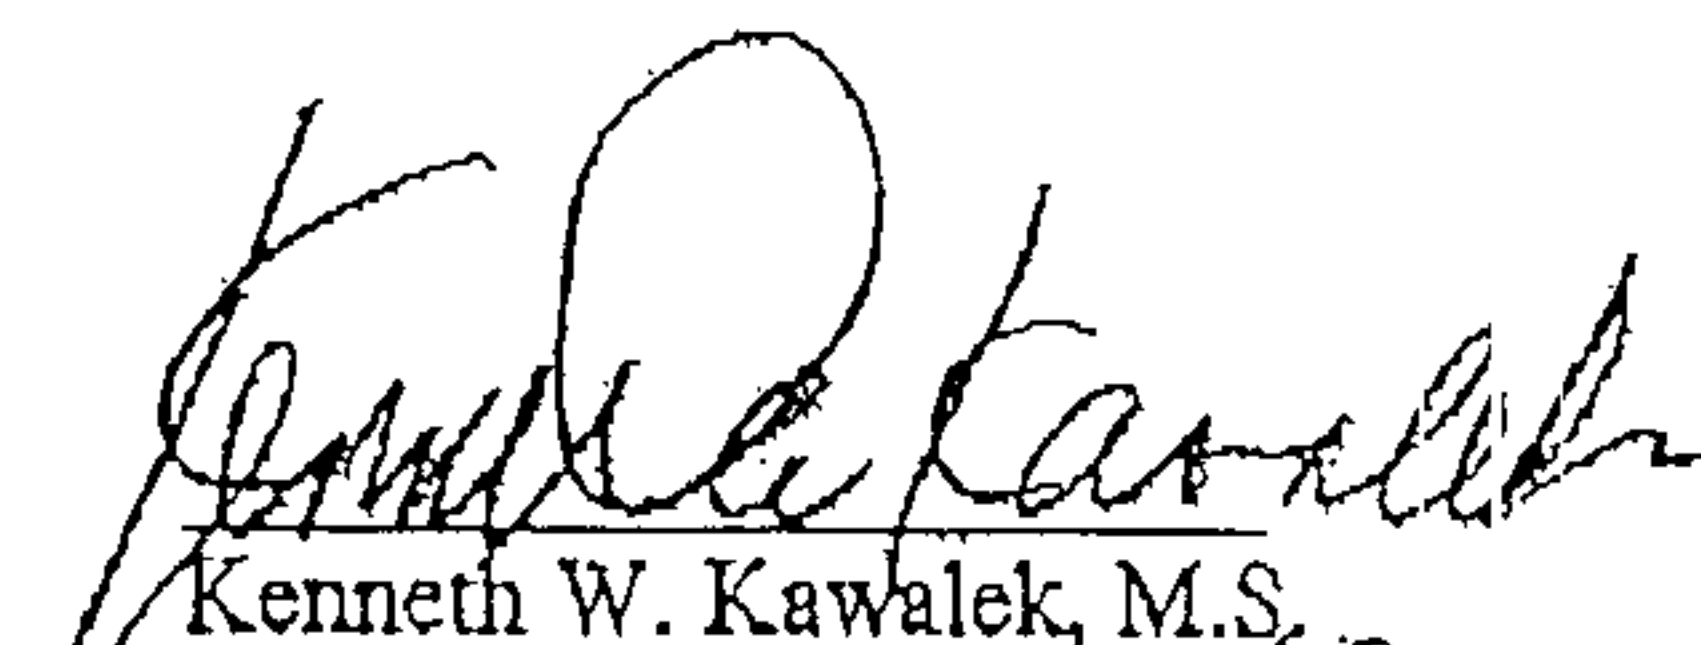  
 Kenneth W. Kawalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 28<sup>th</sup> day of September, 2010.

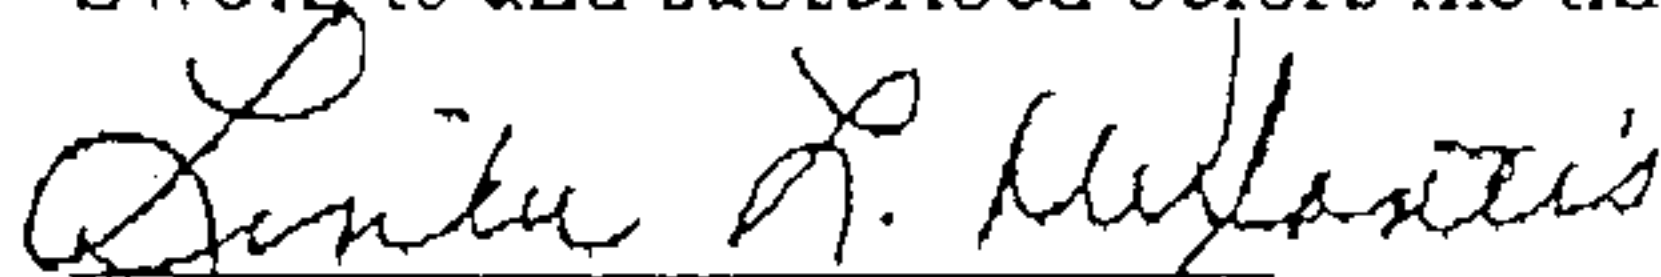  
 Notary

Linda L. Desantis  
 Notary Public, New Jersey  
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable







State of New Jersey  
 OFFICE OF THE ATTORNEY GENERAL  
 DEPARTMENT OF LAW AND PUBLIC SAFETY  
 DIVISION OF STATE POLICE  
 POST OFFICE BOX 7068  
 WEST TRENTON NJ 08628-0068  
 (609) 882-2000

CHRIS CHRISTIE  
 Governor

KIM GUADAGNO  
 Lt. Governor

PAULA T. DOW  
 Attorney General

COLONEL JOSEPH R. FUENTES  
 Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.045 to 0.051 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.


ANALYSIS DATE: 7/21/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F090


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0478 to 0.0485 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 27, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

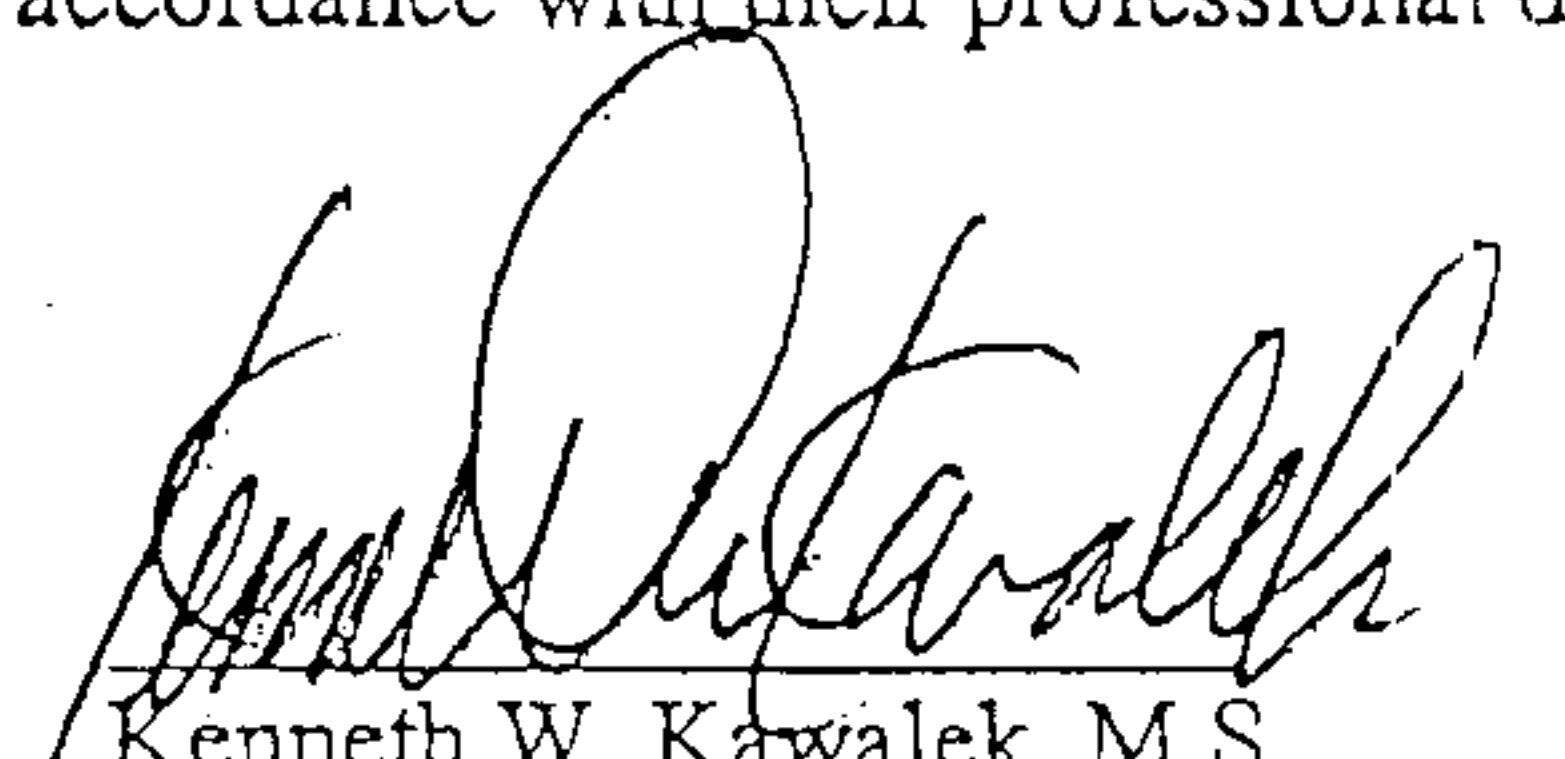  
 Kenneth W. Kawalek, M.S.  
 Assistant Chief Forensic Scientist  
 Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

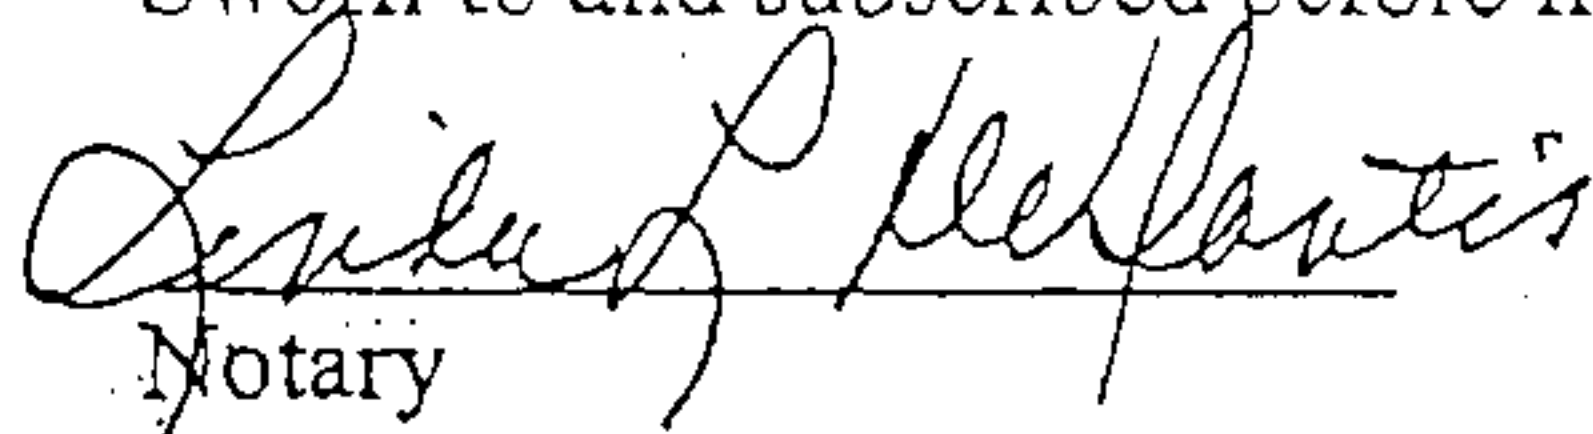
  
 Notary

Linda L. Desantis  
 Notary Public, New Jersey  
 My Commission Expires 8-17-14



New Jersey Is An Equal Opportunity Employer  
 Printed on Recycled Paper and Recyclable



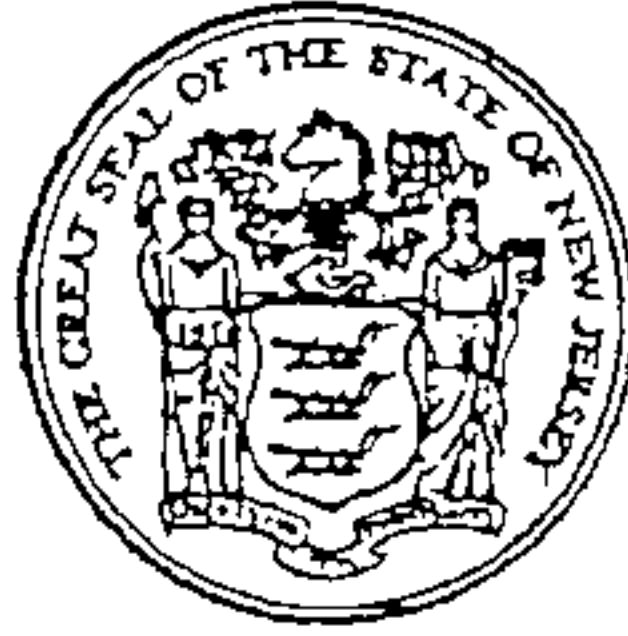

CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lt. Governor

State of New Jersey  
OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

PAULA T. DOW  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

**CERTIFICATION OF ANALYSIS**  
**0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.094 to 0.099 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.

ANALYSIS DATE: 7/22/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11F091

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0968 to 0.0973 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 30, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Kenneth W. Kawalek, M.S.  
Assistant Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

Notary

Linda L. Desantis  
Notary Public, New Jersey  
My Commission Expires 8-17-14



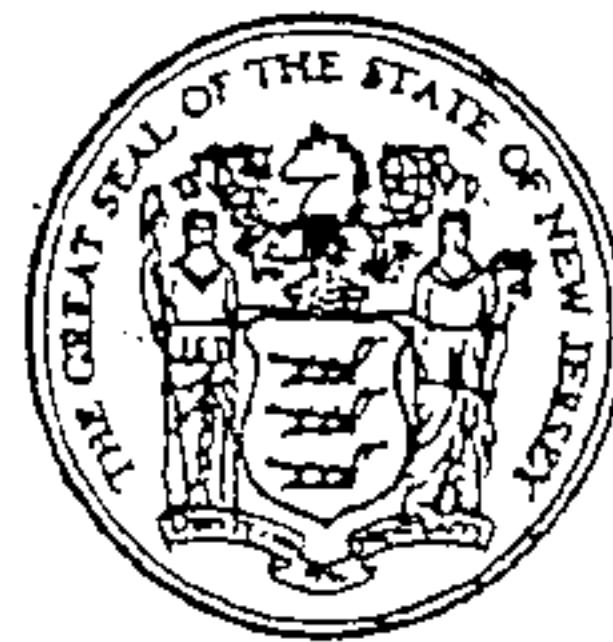

State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON NJ 08628-0068  
(609) 882-2000

CHRIS CHRISTIE  
Governor

KIM GUADAGNO  
Lt. Governor

PAULA T. DOW  
Attorney General

COLONEL JOSEPH R. FUENTES  
Superintendent

CERTIFICATION OF ANALYSIS  
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.188 to 0.199 grams per 100 milliliters of solution.

MANUFACTURER: Drager Safety, Inc.


ANALYSIS DATE: 7/25/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11G092


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1917 to 0.1927 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is July 3, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

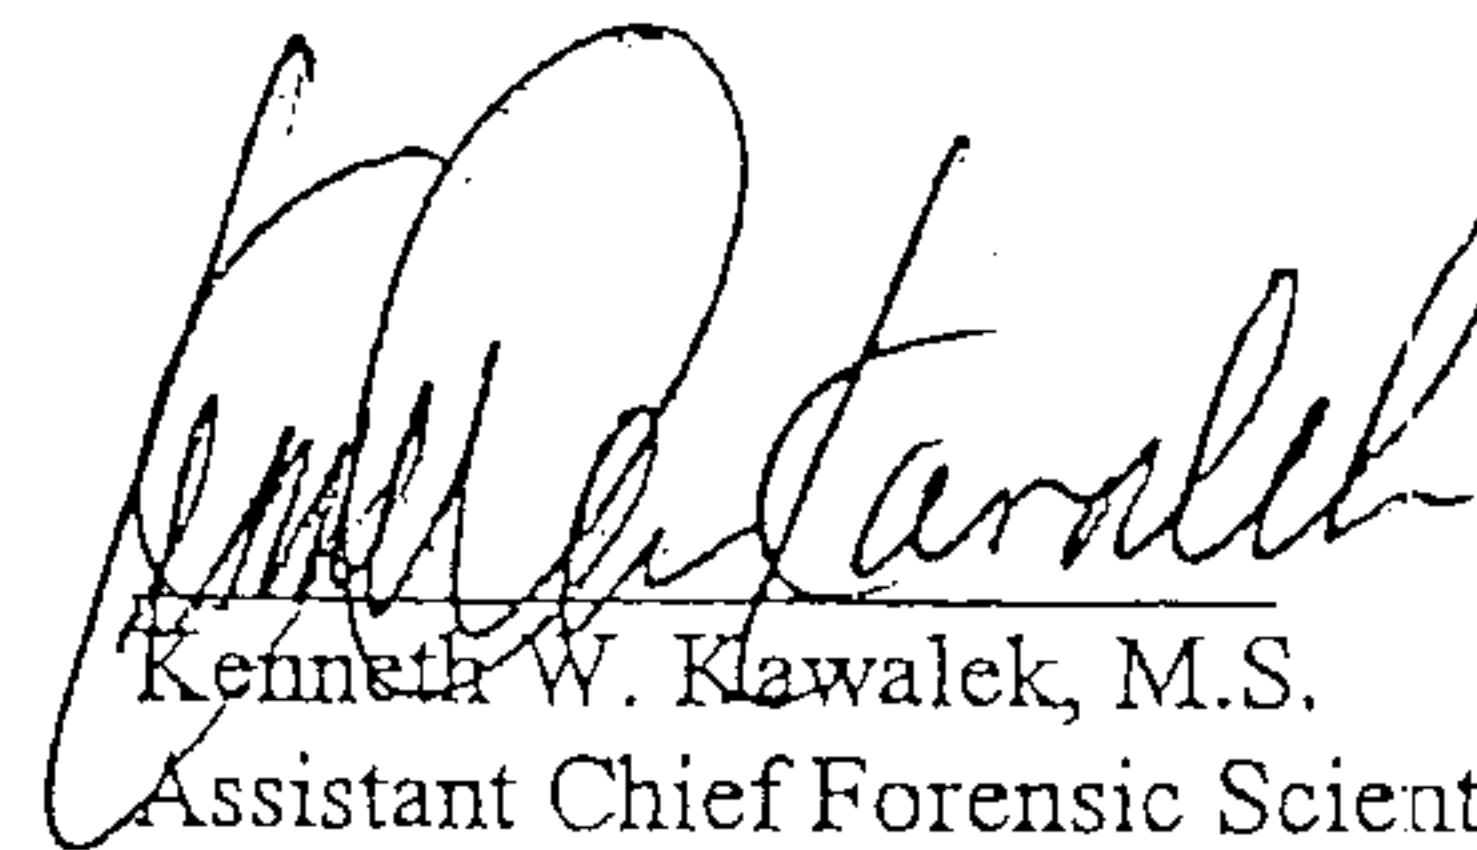  
Kenneth W. Klawalek, M.S.  
Assistant Chief Forensic Scientist  
Division of State Police

Sworn to and subscribed before me this 1<sup>st</sup> day of August, 2011.

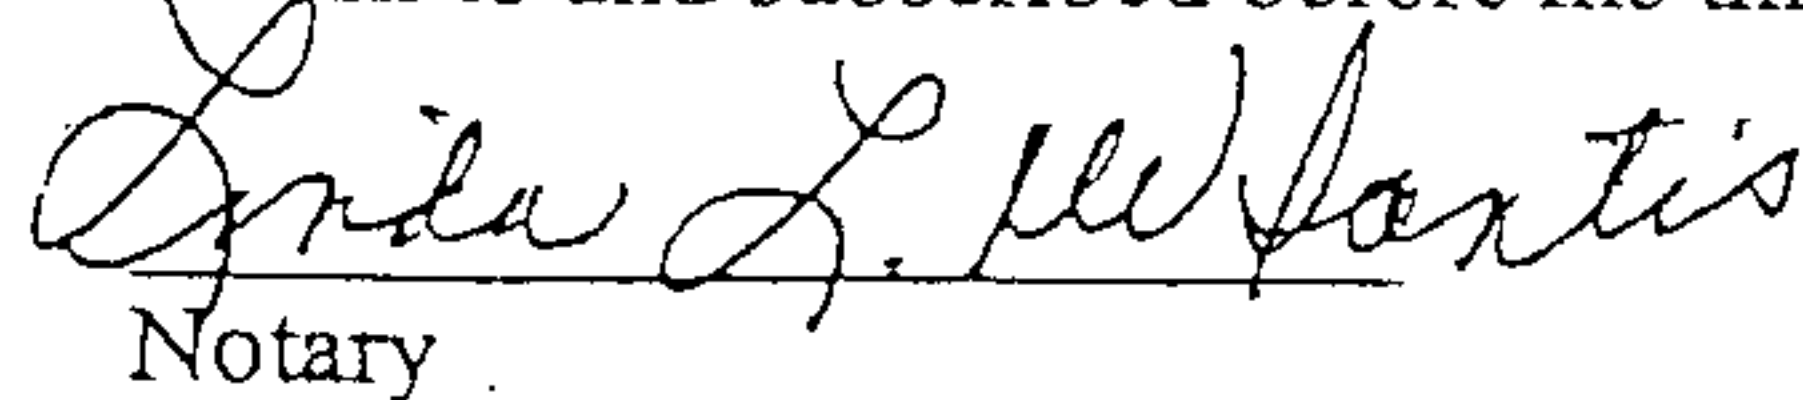  
Notary

Linda L. Desantis  
Notary Public, New Jersey  
My Commission Expires 8-17-14





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON NJ 08628-0068
(609) 882-2000

CHRIS CHRISTIE
Governor

KIM GUADAGNO
Lt. Governor

PAULA T. DOW
Attorney General

COLONEL JOSEPH R. FUENTES
Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.117 to 0.125 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 9/8/2011

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 11H094

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1197 to 0.1207 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-3.4, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 17, 2013.

As Assistant Chief Forensic Scientist of the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at my direction and under my supervision by personnel of, and at, the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Handwritten signature of Kenneth W. Kawalek, M.S.
Kenneth W. Kawalek, M.S.
Assistant Chief Forensic Scientist
Division of State Police

Sworn to and subscribed before me this 12th day of September, 2011.

Handwritten signature of Linda L. D'Amico
Notary



New Jersey Is An Equal Opportunity Employer...
Printed on Recycled Paper and Recyclable



**Dräger**safety

**Alcotest<sup>®</sup> 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:


02-18-2009

SERIAL NUMBER:

AKZL-0146

**Draeger Safety Diagnostics, Inc.**



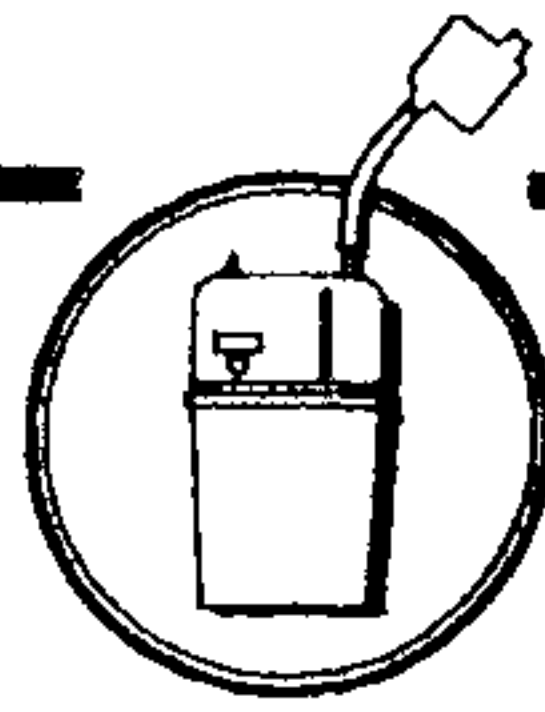

**Dräger**

# CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

**Draeger Safety Diagnostics, Inc.**

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: \_\_\_\_\_

Serial Number:

DDAB-0015

Certification Date

Technician

Re-Certification Due Date

07/30/12

SY

07/30/13

# Dräger

## ALCOTEST® 7110 TEMPERATURE PROBE

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST).

The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

Certification date:

Next Certification due:

DDXKP2-393

07/30/12

07/30/13

Probe Value

104

**Draeger Safety Diagnostics, Inc.**  
Technical Service Department

SY

DEPARTMENT OF  
**Motor and Public Safety**  
 This is to certify that

**Marc W. Dennis**  
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT COURSE IN BREATHALYSE PRACTICE PURSUANT TO CHAPTER 142 OF  
 THE LAWS OF 1964 IN THE OPERATION OF THE Breathalys Coordinator/Instructor  
 A METHOD TO DETERMINE INTOXICATION.  
 GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THE 5th DAY OF November

TWO THOUSAND AND Eight

  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES \_\_\_\_\_

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF  
**Motor and Public Safety**  
 This is to certify that  
**Marc W. Dennis**

New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE **ALCOHOL TEST 7110 MK III-C** A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 26th DAY OF Sept. TWO THOUSAND AND 01

*[Signature]*  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES 8/18 - 8/22/97

Refresher Course

1.	DATE	PLACE	INSTRUCTOR
	11/10/99	O.C.P.A.	Cambria
2.	11-14-01	ACTC	<i>[Signature]</i>
3.	3-17-03	ACTC	<i>[Signature]</i>
4.	10-6-05	ACTC	<i>[Signature]</i>
5.	11-14-07	BCPA	C Potter
6.			
7.			
8.			
9.			

SP-293B (Rev. 4/00)

DEPARTMENT OF  
**Motor and Public Safety**  
 This is to certify that

**Marc W. Dennis**  
 New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF THE LAWS OF 1964 IN THE OPERATION OF THE **ALCOHOL TEST 7110 MK III-C** A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 30th DAY OF April TWO THOUSAND AND Eight

*[Signature]*  
 SUPERINTENDENT  
 NEW JERSEY STATE POLICE

*[Signature]*  
 ATTORNEY GENERAL  
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES 12/1/2005

Refresher Course

1.	DATE	PLACE	INSTRUCTOR
	12-19-07	Ocean Co. PA	Potter
2.	3/12/09	MORRIS CO. PA	<i>[Signature]</i>
3.	2-10-11	SAYREVILLE PD	<i>[Signature]</i>
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 293B (Rev. 07/07)