


Alcotest 7110 Calibration Record

Equipment Alcotest 7110 MKIII-C Serial No.: ARZL-0146
Location: WALL TOWNSHIP POLICE
Calibration File No.: 00886 Calib. Date: 03/25/2015 Calib. No.: 00018
Certification File No.: 00834 Cert. Date: 10/10/2014 Cert. No.: 00014
Linearity File No.: 00835 Lin. Date: 10/10/2014 Lin. No.: 00014
Solution File No.: 00878 Soln. Date: 03/01/2015 Soln. No.: 00173
Sequential File No.: 00886 File Date: 03/25/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXB S3-114
Control Solution %: 0.100% Expires: 09/23/2015
Solution Control Lot: 131123 Bottle No.: 1064

Coordinator
Last Name: DENNIS First Name: MARC MI: W.
Signature: SGT. R. Dennis #5925 Badge No.: 5925
Date: 03/25/2015

*Black Key Temperature Probe Serial.....# DDXK P2-376 (MAD)
*Digital NIST Temperature Measuring System Serial.....# 130754749 (MAD)

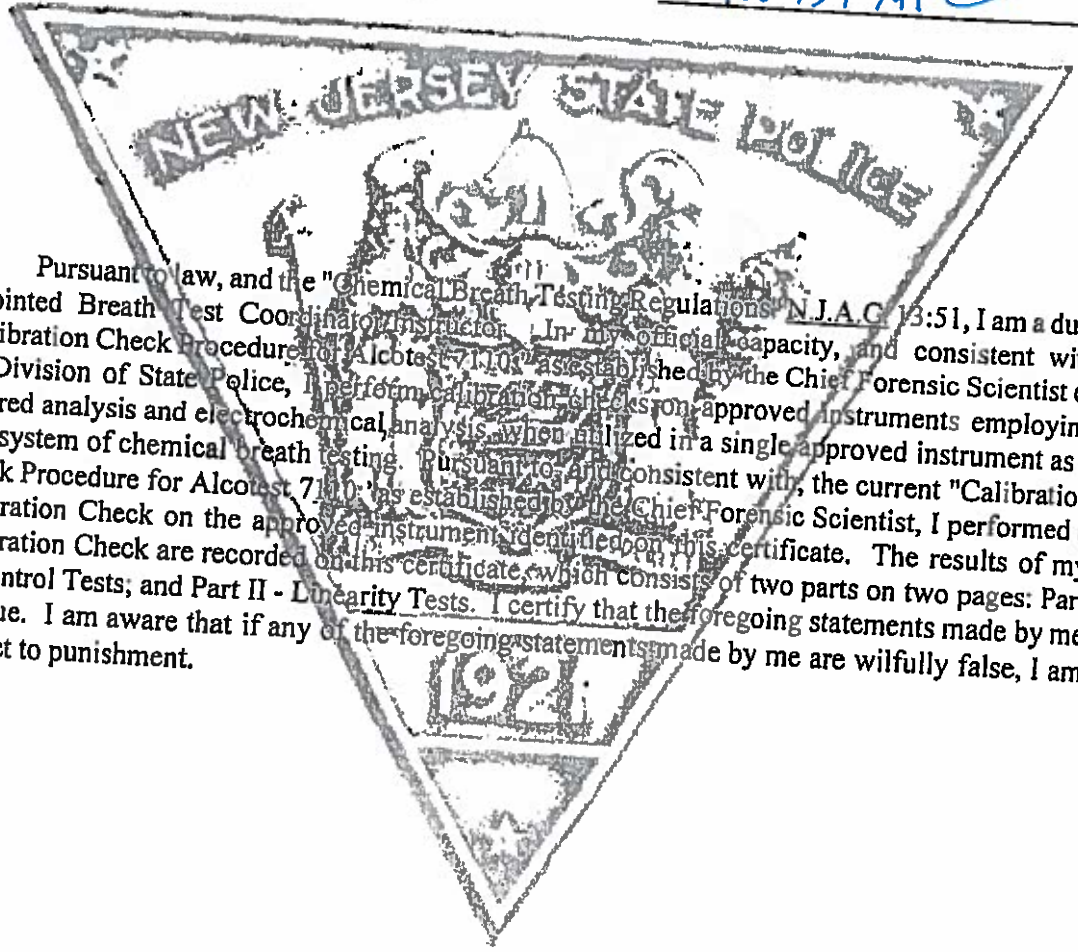

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARZL-0146
Location:	WALL TOWNSHIP POLICE	Calib. No.:	00018
Calibration File No.:	00886	Cert. Date:	03/25/2015
Certification File No.:	00887	Lin. Date:	10/10/2014
Linearity File No.:	00835	Soln. Date:	03/01/2015
Solution File No.:	00878	File Date:	03/25/2015
Sequential File No.:	00887		
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXB S3-114
Solution Control Lot:	131123	Expires:	09/23/2015
		Bottle No.:	1064

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:37S	14.370 °C	
Control 1 EC	0.100%	13:37S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	13:37S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:38S		
Control 2 EC	0.098%	13:39S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:39S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:40S		
Control 3 EC	0.099%	13:40S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	13:40S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:41S	14.410 °C	

All tests within acceptable tolerance.

Coordinator

Last Name: DENNIS

Signature: SGT [Signature]


First Name: MARC

Badge No.: 5925

Date: 03/25/2015

MI: W.

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

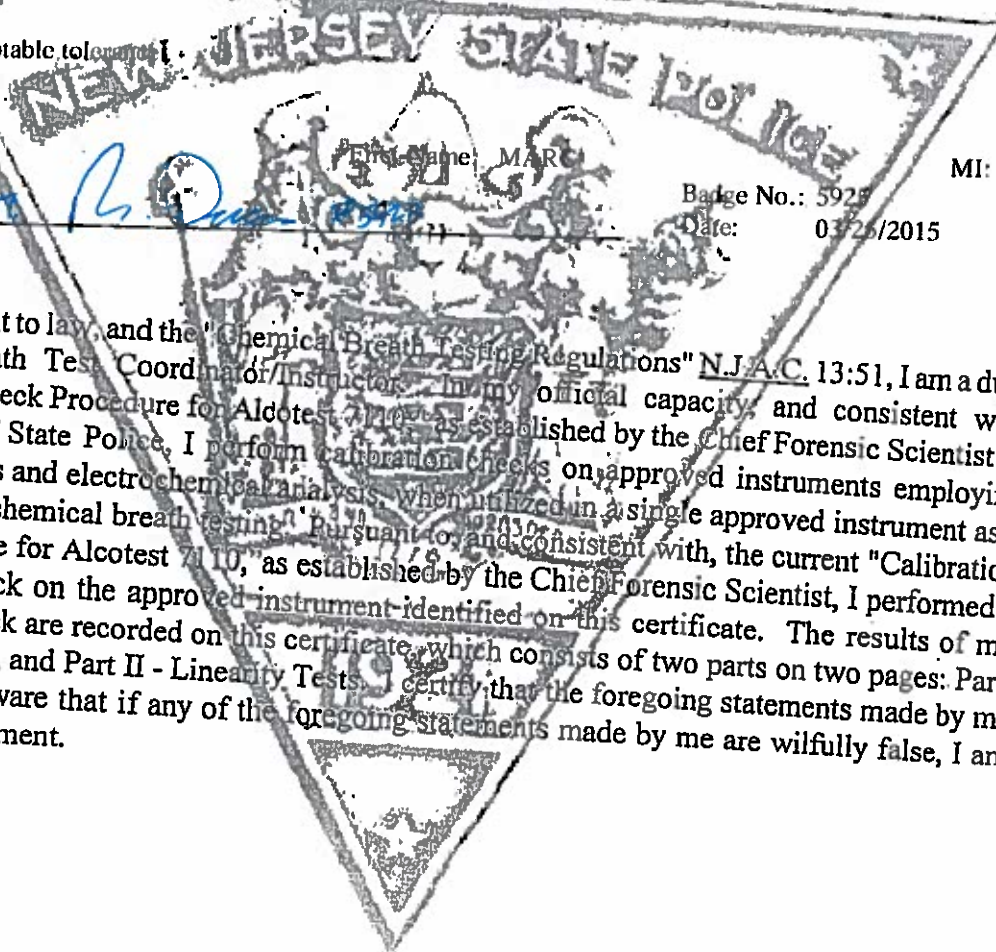

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment

Alcotest 7110 MKIII-C
 Location: WALL TOWNSHIP POLICE
 Calibration File No.: 00886
 Certification File No.: 00887
 Linearity File No.: 00888
 Solution File No.: 00878
 Sequential File No.: 00888

Calib. Date: 03/25/2015
 Cert. Date: 03/25/2015
 Lin. Date: 03/25/2015
 Soln. Date: 03/01/2015
 File Date: 03/25/2015

Serial No.: ARZL-0146

Calib. No.: 00018
 Cert. No.: 00015
 Lin. No.: 00015
 Soln. No.: 00173

Calibrating Unit: WET
 Control Solution %: 0.040%
 Solution Control Lot: 13I120

Model No.: CU-34

Serial No.: DDXD S3-0186
 Expires: 09/13/2015
 Bottle No.: 0100

Calibrating Unit: WET
 Control Solution %: 0.080%
 Solution Control Lot: 13I121

Model No.: CU-34

Serial No.: DDXD S3-0188
 Expires: 09/16/2015
 Bottle No.: 0400

Calibrating Unit: WET
 Control Solution %: 0.160%
 Solution Control Lot: 14H131

Model No.: CU-34

Serial No.: DDXD S3-0191
 Expires: 08/05/2016
 Bottle No.: 0758

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:56S	14:56 D (P)	
Control 1 EC	0.041%	13:56S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.041%	13:56S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:58S		
Control 2 EC	0.041%	13:59S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.040%	13:59S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:00S		
Control 3 EC	0.080%	14:01S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.080%	14:01S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:02S		
Control 4 EC	0.080%	14:03S	33.9°C	*** TEST PASSED ***
Control 4 IR	0.079%	14:03S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:05S		
Control 5 EC	0.157%	14:05S	33.9°C	*** TEST PASSED ***
Control 5 IR	0.157%	14:05S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:07S		
Control 6 EC	0.158%	14:08S	33.9°C	*** TEST PASSED ***
Control 6 IR	0.158%	14:08S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:09S	15:09 D (P)	

All tests within acceptable tolerance.

Coordinator

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: SGT. R. Dennis 25925

Badge No.: 5925

Date: 03/25/2015

Calibrating Unit New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARZL-0146
Location:	WALL TOWNSHIP POLICE	
Calibration File No.:	00886	Calib. No.: 00018
Certification File No.:	00887	Cert. No.: 00015
Linearity File No.:	00888	Lin. No.: 00015
Solution File No.:	00889	Soln. No.: 00174
Sequential File No.:	00889	
	Calib. Date: 03/25/2015	
	Cert. Date: 03/25/2015	
	Lin. Date: 03/25/2015	
	Soln. Date: 03/25/2015	
	File Date: 03/25/2015	

Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXB S3-114
Solution Control Lot:	14D129	Expires: 04/29/2016
		Bottle No.: 0134

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	15:15S	16:15D ☺	
Control 1 EC	0.101%	15:16S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	15:16S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:17S		
Control 2 EC	0.101%	15:17S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.102%	15:17S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:18S		
Control 3 EC	0.101%	15:19S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.101%	15:19S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	15:20S	14:20D ☺	

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number DDWJ P2-283 ☺

Changed By:

Last Name: DENNIS

First Name: MARC

MI: W.

Signature: SGT. [Signature] #5925

Badge No.: 5925

Date: 03/25/2015



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDXDS3-0186

Certification Date

9-22-14

Technician

BC

Re-Certification Due Date

9-22-15



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDXDS3-0188

Certification Date

9-22-14

Technician

BC

Re-Certification Due Date

9-22-15



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to Calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger Safety Diagnostics, Inc.

Model: ALCOTEST® CU34

Model: MARK IIA

Other: _____

Serial Number:

DDXDS3-0191

Certification Date

9-19-14

Technician

BC

Re-Certification Due Date

9-19-15

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDXK P2-376

Certification date:

9-2-14

Next Certification due:

9-2-15

Probe Value

106

Dräger Safety Diagnostics, Inc.
Technical Service Department

BC



Calibration complies with ISO/IEC 17025, ANSI/NCSL Z540-1, and 9001



Calibration Certificate No. 1750.01

Cert. No.: 4000-5574134

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087
Instrument Identification:

Model: 61220-601 S/N: 130754749 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-179	A48240		
Thermistor Module	A17118	2/13/14	1000332071
Temperature Probe	128	2/20/14	6-B48Z9-30-1
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A17118	2/13/14	1000332071
Temperature Probe	3039	2/20/14	6-B48Z9-1-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Module	A27129	10/25/14	1000346002
Temperature Probe	5202	11/30/14	15-B15PW-1-1
Temperature Calibration Bath TC-275	B16388		
Digital Thermometer	B16815	8/12/14	1000341967
PRT Temperature Probe	02022	8/14/15	B3812004

Certificate Information:

Technician: 88 Procedure: CAL-08 Cal Date: 12/12/13 Cal Due: 12/12/15
Test Conditions: 24.0°C 33.0 %RH 1033 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.001	0.001	Y	-0.049	0.051	0.013	3.8:1
°C		N.A.		24.999	25.001	Y	24.949	25.049	0.023	2.2:1
°C		N.A.		50.003	50.000	Y	49.953	50.053	0.014	3.6:1
°C		N.A.		100.001	99.999	Y	99.951	100.051	0.018	2.8:1

This instrument was calibrated using instruments traceable to National Institute of Standards and Technology. A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Dpt=MM/DD/YY

Nicol Rodriguez
Nicol Rodriguez, Quality Manager

Aaron Justice
Aaron Justice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change Rds, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 4455 Rox Road Friendswood, TX 77546 USA
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01905-2008-AQ-HOU-RuA.
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/24/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 13I123

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1186 to 0.1192 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 23, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of October, 2013.

Sandra L. de Santos
 Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/25/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 131120

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0484 to 0.0489 grams per 100 milliliters of solution.


This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 13, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28th day of October, 2013.

Linda L. W. Panteis
 Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.

ANALYSIS DATE: 10/31/2013

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 131121

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0959 to 0.0971 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is September 16, 2015.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 1st day of November, 2013.

Mary E. McLaughlin
 Notary

MARY ELIZABETH MCLAUGHLIN
 NOTARY PUBLIC OF NEW JERSEY
 MY COMMISSION EXPIRES 12-24-2013



"An Internationally Accredited Agency"

New Jersey is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 8/14/2014

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 14H131


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1925 to 0.1944 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 5, 2016.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

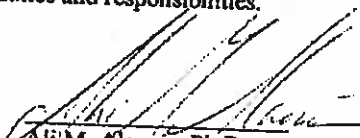
 Ali M. Alaouie, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18th day of August, 2014.


 Notary
MARY ELIZABETH MCLAUGHLIN
 ID # 2052180
 NOTARY PUBLIC
 STATE OF NEW JERSEY
 My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable





State of New Jersey
 OFFICE OF THE ATTORNEY GENERAL
 DEPARTMENT OF LAW AND PUBLIC SAFETY
 DIVISION OF STATE POLICE
 POST OFFICE BOX 7068
 WEST TRENTON, NJ 08628-0068
 (609) 882-2000

CHRIS CHRISTIE
 Governor

KIM GUADAGNO
 Lt. Governor

JOHN J. HOFFMAN
 Acting Attorney General

COLONEL JOSEPH R. FUENTES
 Superintendent

CERTIFICATION OF ANALYSIS
0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Dräger Safety, Inc.

ANALYSIS DATE: 5/06/2014

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 14D129

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1208 to 0.1217 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is April 29, 2016.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaoui, Ph.D.
 Research Scientist
 NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 06 day of May, 2014.

Joseph R. Fuentes
 Notary

Lynia L. Gonzalez
 Notary Public, New Jersey
 My Commission Expires 6-17-14



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
 Printed on Recycled Paper and Recyclable



Dräger

Alcotest® 7110 MKIII-C

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

4-8-14

SERIAL NUMBER:

ARZL-D146

Draeger Safety Diagnostics, Inc.

BL



Dräger

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger Safety Diagnostics, Inc.

- Model: ALCOTEST® CU34
- Model: MARK IIA
- Other: _____

Serial Number:

DDXB53-114

Certification Date

1-30-15

Technician

BC

Re-Certification Due Date

1-30-16

Dräger

ALCOTEST® 7110 TEMPERATURE PROBE

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest® 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your State Specification. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest® 7110.

Serial Number Temp. Probe

DDWSP2-283

Certification date:

1-30-15

Next Certification due:

1-30-16

Probe Value

103

Draeger Safety Diagnostics, Inc.
Technical Service Department

BC

DEPARTMENT OF
Traffic and Public Safety

This is to certify that
Marc W. Dennis
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT GENERAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF THE LAWS OF 1944 IN THE OPERATION OF THE **7110 MK III-C** BREATHANALYZER
A METHOD TO DETERMINE INTOXICATION

CITIZEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 26th DAY OF Sept.
TWO THOUSAND AND 01

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 8/18 - 8/22/97

Refreshers Course

DATE	PLACE	INSTRUCTOR
1. 11/10/99	O.C.P.A.	Cambrila
2. 11-14-01	AGTC	<i>[Signature]</i>
3. 7-17-03	AGTC	<i>[Signature]</i>
4. 10-6-05	AGTC	<i>[Signature]</i>
5. 11-14-07	OCPA	C. Potter
6.		
7.		
8.		
9.		

SP-293B (Rev. 4/00)

DEPARTMENT OF
Traffic and Public Safety

This is to certify that
Marc W. Dennis
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT GENERAL BREATH ANALYSIS PURSUANT TO CHAPTER 142 OF THE LAWS OF 1944 IN THE OPERATION OF THE **7110 MK III-C** BREATHANALYZER
A METHOD TO DETERMINE INTOXICATION

CITIZEN UNDER MY HAND AT TRENTON, NEW JERSEY, THIS 30th DAY OF April
TWO THOUSAND AND Eight

[Signature]
SUPERINTENDENT
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES 12/1/2005

Refreshers Course

DATE	PLACE	INSTRUCTOR
1. 12-19-07	Ocean Co. PA	Potter
2. 3/12/09	MORRIS CO. PA	<i>[Signature]</i>
3. 2-16-11	SAYREVILLE PD	<i>[Signature]</i>
4. 11/19/13	S.C.E.S.T.A.	<i>[Signature]</i>
5.		
6.		
7.		
8.		
9.		

S.P. 293B (Rev. 07/07)

DEPARTMENT OF
Law and Public Safety
 This is to certify that

Marc W. Dennis
 New Jersey State Police



IS QUALIFIED AND COMPETENT TO CONDUCT COURSE WITH OFFICERS PURSUANT TO CHAPTER 143 OF
 THE LAWS OF 1964 IN THE OPERATION OF THE BREATH TEST METHOD PURSUANT TO CHAPTER 143 OF
 A METHOD TO DETERMINE INTOXICATION.

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY, this 5th DAY OF November
 TWO THOUSAND AND Eight

[Signature]
 SUPERINTENDENT
 NEW JERSEY STATE POLICE

[Signature]
 ATTORNEY GENERAL
 STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1.		
2.		
3.		
4.		
5.		
6.		
7.		
8.		
9.		

S.P. 2938 (Rev. 07/07)