

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0037
Location:	WALL TOWNSHIP POLICE		
Calibration File No.:	00393	Calib. Date:	03/29/2011
Certification File No.:	00394	Cert. No.:	00011
Linearity File No.:	00395	Lin. Date:	03/29/2011
Solution File No.:	00480	Lin. No.:	00007
Sequential File No.:	00480	Soln. Date:	08/13/2011
		Soln. No.:	00094
		File Date:	08/13/2011
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXB S3-114
Solution Control Lot:	10L084	Expires:	12/16/2012
		Bottle No.:	0768

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	13:19D		
Control 1 EC	0.098%	13:20D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	13:20D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20D		
Control 2 EC	0.096%	13:21D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	13:21D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:22D		
Control 3 EC	0.096%	13:22D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	13:22D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:23D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: LISTER

First Name: EDWARD

MI: J

Signature: _____

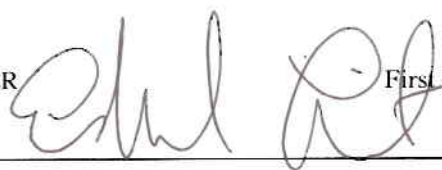

Badge No.: 142

Date: 08/13/2011