

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.: ARZL-0146
Location:	WALL TOWNSHIP POLICE	
Calibration File No.:	00459	Calib. Date: 03/07/2012
Certification File No.:	00460	Calib. No.: 00010
Linearity File No.:	00461	Cert. Date: 03/07/2012
Solution File No.:	00479	Cert. No.: 00008
Sequential File No.:	00479	Lin. Date: 03/07/2012
		Lin. No.: 00008
		Soln. Date: 05/14/2012
		Soln. No.: 00089
		File Date: 05/14/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDXB S3-114
Solution Control Lot:	11H094	Expires: 08/17/2013
		Bottle No.: 0322

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	14:00D		
Control 1 EC	0.100%	14:00D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	14:00D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:01D		
Control 2 EC	0.098%	14:02D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	14:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:03D		
Control 3 EC	0.099%	14:03D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	14:03D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	14:04D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: ~~COSTANTINI~~

First Name: JASON

MI: R

Signature: _____

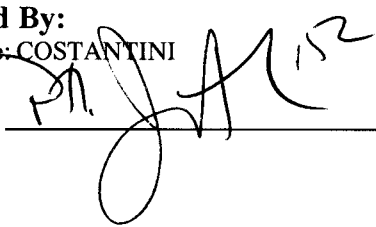

Badge No.: 152

Date: 05/14/2012