

Calibrating Unit

New Standard Solution Report

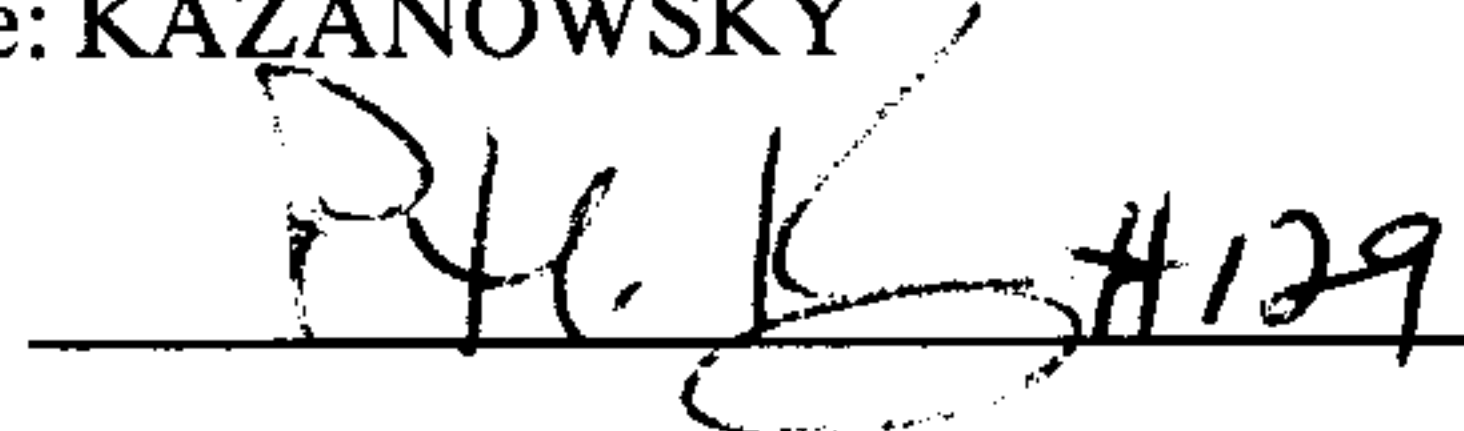
Equipment	Alcotest 7110 MKIII-C	Serial No.: ARZL-0146
Location:	WALL TOWNSHIP POLICE	
Calibration File No.:	00527	Calib. Date: 09/04/2012
Certification File No.:	00528	Calib. No.: 00011
Linearity File No.:	00529	Cert. Date: 09/04/2012
Solution File No.:	00538	Cert. No.: 00009
Sequential File No.:	00538	Lin. Date: 09/04/2012
		Lin. No.: 00009
		Soln. Date: 10/01/2012
		Soln. No.: 00099
		File Date: 10/01/2012
Calibrating Unit:	WET	Model No.: CU-34
Control Solution %:	0.100%	Serial No.: DDAB-0015
Solution Control Lot:	11H094	Expires: 08/17/2013
		Bottle No.: 0265

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	16:59D		
Control 1 EC	0.100%	16:59D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	16:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:00D		
Control 2 EC	0.098%	17:01D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	17:01D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:01D		
Control 3 EC	0.098%	17:02D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	17:02D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	17:03D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KAZANOWSKY	First Name: PTL	MI: A
Signature: <u></u>	Badge No.: 129	Date: 10/01/2012