

# Calibrating Unit

## New Standard Solution Report

<b>Equipment</b>	Alcotest 7110 MKIII-C	Serial No.:	ARZL-0146
Location:	WALL TOWNSHIP POLICE		
Calibration File No.:	00527	Calib. Date:	09/04/2012
Certification File No.:	00528	Cert. Date:	09/04/2012
Linearity File No.:	00529	Lin. Date:	09/04/2012
Solution File No.:	00541	Soln. Date:	10/19/2012
Sequential File No.:	00541	File Date:	10/19/2012

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDAB-0015
Control Solution %:	0.100%			Expires:	08/17/2013
Solution Control Lot:	11H094			Bottle No.:	0264

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:51D		
Control 1 EC	0.100%	09:52D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	09:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:53D		
Control 2 EC	0.099%	09:54D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:54D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54D		
Control 3 EC	0.098%	09:55D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:56D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: KAZANOWSKY

First Name: PTL

MI: A

Signature: \_\_\_\_\_

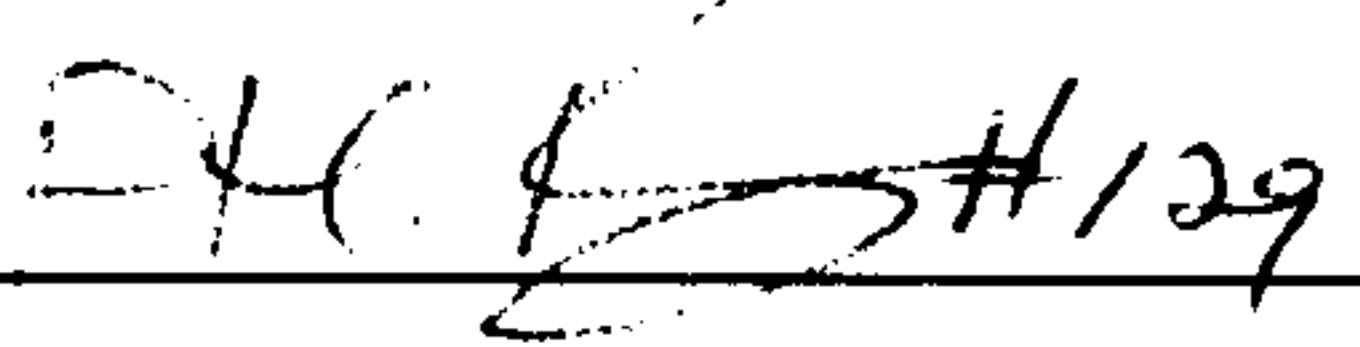

Badge No.: 129

Date: 10/19/2012