

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0037
Location:	WALL TOWNSHIP POLICE		
Calibration File No.:	00899	Calib. Date:	08/28/2013
Certification File No.:	00900	Cert. Date:	08/28/2013
Linearity File No.:	00901	Lin. Date:	08/28/2013
Solution File No.:	00950	Soln. Date:	11/08/2013
Sequential File No.:	00950	File Date:	11/08/2013

Calibrating Unit:	WET	Model No.:	CU-34	Serial No.:	DDAB-0015
Control Solution %:	0.100%			Expires:	06/17/2015
Solution Control Lot:	13F114			Bottle No.:	1108

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	23:49S		
Control 1 EC	0.101%	23:50S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.100%	23:50S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:50S		
Control 2 EC	0.099%	23:51S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	23:51S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:51S		
Control 3 EC	0.099%	23:52S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	23:52S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	23:53S		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: OHALLORAN

First Name: SEAN

MI: P

Signature: _____

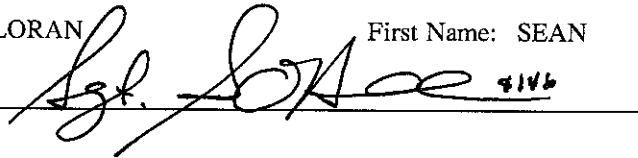

Badge No.: 146

Date: 11/08/2013