

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0037
Location: WALL TOWNSHIP POLICE
Calibration File No.: 01062 Calib. Date: 05/06/2014 Calib. No.: 00023
Certification File No.: 01063 Cert. Date: 05/06/2014 Cert. No.: 00015
Linearity File No.: 01064 Lin. Date: 05/06/2014 Lin. No.: 00015
Solution File No.: 01103 Soln. Date: 06/11/2014 Soln. No.: 00186
Sequential File No.: 01103 File Date: 06/11/2014

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXB S3-113
Control Solution %: 0.100% Expires: 09/10/2015
Solution Control Lot: 131119 Bottle No.: 0295

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	05:41D		
Control 1 EC	0.097%	05:42D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	05:42D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:42D		
Control 2 EC	0.097%	05:43D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	05:43D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:43D		
Control 3 EC	0.098%	05:44D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.098%	05:44D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	05:45D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: JENNINGS

First Name: ERIC

MI: R

Signature: _____

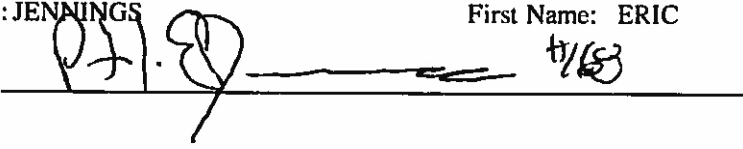

6/11/14

Badge No.: 168

Date: 06/11/2014