

# Calibrating Unit

## New Standard Solution Report

|                         |                       |                         |
|-------------------------|-----------------------|-------------------------|
| <b>Equipment</b>        | Alcotest 7110 MKIII-C | Serial No.: ARZL-0146   |
| Location:               | WALL TOWNSHIP POLICE  |                         |
| Calibration File No.:   | 00995                 | Calib. Date: 09/08/2015 |
| Certification File No.: | 00996                 | Calib. No.: 00019       |
| Linearity File No.:     | 00997                 | Cert. Date: 09/08/2015  |
| Solution File No.:      | 01102                 | Cert. No.: 00016        |
| Sequential File No.:    | 01102                 | Lin. Date: 09/08/2015   |
|                         |                       | Lin. No.: 00016         |
|                         |                       | Soln. Date: 02/12/2016  |
|                         |                       | Soln. No.: 00208        |
|                         |                       | File Date: 02/12/2016   |

|                       |        |            |       |             |            |
|-----------------------|--------|------------|-------|-------------|------------|
| Calibrating Unit:     | WET    | Model No.: | CU-34 | Serial No.: | DDAB-0015  |
| Control Solution %:   | 0.100% |            |       | Expires:    | 01/05/2017 |
| Solution Control Lot: | 16A150 |            |       | Bottle No.: | 0513       |

| Function          | Result<br>%BAC | Time<br>HH:MM | Temperature<br>Simulator (°C) | Comment(s)<br>or Error(s) |
|-------------------|----------------|---------------|-------------------------------|---------------------------|
| Ambient Air Blank | 0.000%         | 22:12S        |                               |                           |
| Control 1 EC      | 0.100%         | 22:13S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 1 IR      | 0.101%         | 22:13S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 22:14S        |                               |                           |
| Control 2 EC      | 0.100%         | 22:15S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 2 IR      | 0.099%         | 22:15S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 22:15S        |                               |                           |
| Control 3 EC      | 0.100%         | 22:16S        | 34.0°C                        | *** TEST PASSED ***       |
| Control 3 IR      | 0.101%         | 22:16S        | 34.0°C                        | *** TEST PASSED ***       |
| Ambient Air Blank | 0.000%         | 22:17S        |                               |                           |

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


**Changed By:**

Last Name: BALDINO

First Name: ANDREW

MI: M

Signature: \_\_\_\_\_

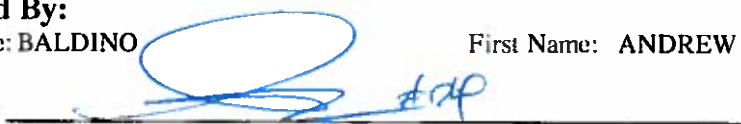

Badge No.: 174

Date: 02/12/2016