

# Alcotest 7110 Calibration Record

## Equipment

Alcotest 7110 MKIII-C	Serial No.: ARZL-0146
Location: WALL TOWNSHIP POLICE	
Calibration File No.: 01453	Calib. Date: 06/15/2018
Certification File No.: 01405	Calib. No.: 00029
Linearity File No.: 01406	Cert. Date: 12/26/2017
Solution File No.: 01452	Cert. No.: 00024
Sequential File No.: 01453	Lin. Date: 12/26/2017
	Lin. No.: 00024
	Soln. Date: 06/13/2018
	Soln. No.: 00270
	File Date: 06/15/2018
Calibrating Unit: WET	Model No.: CU-34
Control Solution %: 0.100%	Serial No.: DDAB-0014
Solution Control Lot: 16270	Expires: 10/10/2018
	Bottle No.: 1311

## Coordinator

Last Name: KOZIEL First Name: BARTLOMIEJ MI:

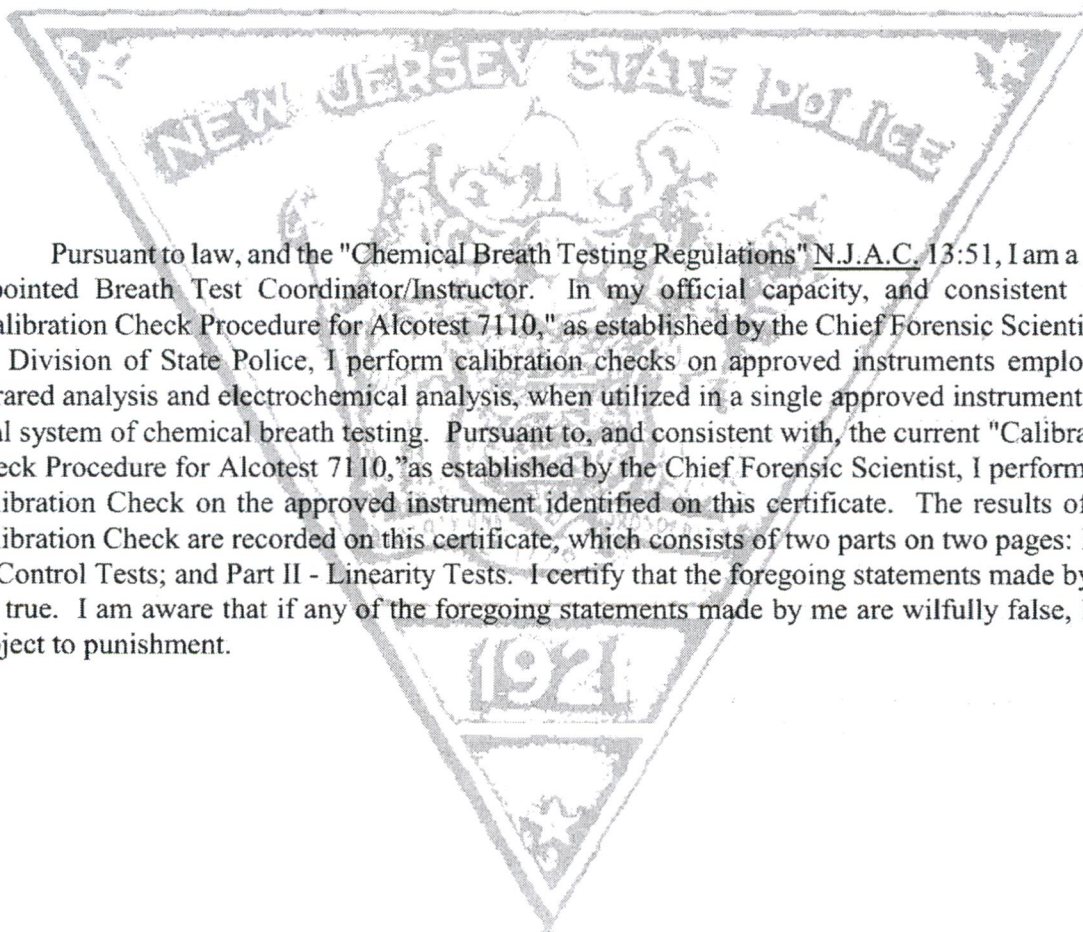
Signature: T. I. B. Koziel # 7041 Badge No.: 7041

Date: 06/15/2018

\*Black Key Temperature Probe Serial.....# DDUJ P2-003 (BK)

\*Digital NIST Temperature Measuring System Serial.....# 170297888 (BK)

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.



# Alcotest 7110 Calibration Certificate

## Part I - Control Tests

### Equipment

Alcotest 7110 MKIII-C  
Location: WALL TOWNSHIP POLICE  
Serial No.: ARZL-0146  
Calibration File No.: 01453  
Calib. Date: 06/15/2018  
Calib. No.: 00029  
Certification File No.: 01454  
Cert. Date: 06/15/2018  
Cert. No.: 00025  
Linearity File No.: 01406  
Lin. Date: 12/26/2017  
Lin. No.: 00024  
Solution File No.: 01452  
Soln. Date: 06/13/2018  
Soln. No.: 00270  
Sequential File No.: 01454  
File Date: 06/15/2018  
Calibrating Unit: WET  
Model No.: CU-34  
Serial No.: DDAB-0014  
Control Solution %: 0.100%  
Expires: 10/10/2018  
Solution Control Lot: 16270  
Bottle No.: 1311

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:45D		
Control 1 EC	0.100%	10:46D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	10:46D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:47D		
Control 2 EC	0.099%	10:47D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.100%	10:47D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:48D		
Control 3 EC	0.099%	10:49D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	10:49D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:50D		

All tests within acceptable tolerance.

### Coordinator

Last Name: KOZIEL

First Name: BARTLOMIEJ

MI:

Signature: \_\_\_\_\_

Badge No.: 7041

Date: 06/15/2018

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.



# Alcotest 7110 Calibration Certificate

## Part II - Linearity Tests

### Equipment

Alcotest 7110 MKIII-C  
Location: WALL TOWNSHIP POLICE  
Serial No.: ARZL-0146  
Calibration File No.: 01453 Calib. Date: 06/15/2018 Calib. No.: 00029  
Certification File No.: 01454 Cert. Date: 06/15/2018 Cert. No.: 00025  
Linearity File No.: 01455 Lin. Date: 06/15/2018 Lin. No.: 00025  
Solution File No.: 01452 Soln. Date: 06/13/2018 Soln. No.: 00270  
Sequential File No.: 01455 File Date: 06/15/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0196  
Control Solution %: 0.040% Expires: 08/10/2019  
Solution Control Lot: 17240 Bottle No.: 1391

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDWE S3-0205  
Control Solution %: 0.080% Expires: 08/15/2019  
Solution Control Lot: 17250 Bottle No.: 0308

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDRF S3-0011  
Control Solution %: 0.160% Expires: 08/21/2019  
Solution Control Lot: 17260 Bottle No.: 0636

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:00D		
Control 1 EC	0.040%	11:00D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.039%	11:00D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:02D		
Control 2 EC	0.038%	11:02D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.038%	11:02D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:04D		
Control 3 EC	0.079%	11:04D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.079%	11:04D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:06D		
Control 4 EC	0.079%	11:06D	33.9°C	*** TEST PASSED ***
Control 4 IR	0.078%	11:06D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:08D		
Control 5 EC	0.159%	11:08D	33.9°C	*** TEST PASSED ***
Control 5 IR	0.158%	11:08D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:10D		
Control 6 EC	0.156%	11:11D	33.9°C	*** TEST PASSED ***
Control 6 IR	0.157%	11:11D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:12D		

All tests within acceptable tolerance.

### Coordinator

Last Name: KOZIEL

First Name: BARTLOMIEJ

MI:

Signature: \_\_\_\_\_

*T. I. B. Koziel* # 7041

Badge No.: 7041

Date: 06/15/2018

# Calibrating Unit

## New Standard Solution Report

**Equipment**

Alcotest 7110 MKIII-C  
Location: WALL TOWNSHIP POLICE  
Serial No.: ARZL-0146  
Calibration File No.: 01453 Calib. Date: 06/15/2018 Calib. No.: 00029  
Certification File No.: 01454 Cert. Date: 06/15/2018 Cert. No.: 00025  
Linearity File No.: 01455 Lin. Date: 06/15/2018 Lin. No.: 00025  
Solution File No.: 01456 Soln. Date: 06/15/2018 Soln. No.: 00271  
Sequential File No.: 01456 File Date: 06/15/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0014  
Control Solution %: 0.100% Expires: 12/11/2019  
Solution Control Lot: 17420 Bottle No.: 1115

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	12:18D		
Control 1 EC	0.100%	12:19D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	12:19D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:19D		
Control 2 EC	0.100%	12:20D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.101%	12:20D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:21D		
Control 3 EC	0.100%	12:21D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.101%	12:21D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:22D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with  
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDXK P2-369 (BK)

**Changed By:**

Last Name: KOZIEL

First Name: BARTLOMIEJ

MI:

Signature: T. I. B. Koziel # 7041

Badge No.: 7041

Date: 06/15/2018



**Dräger**

**Alcotest® 7110 MKIII-C**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 MKIII-C has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48864 and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your State Specifications.

Certification Date:

9-2-16

SERIAL NUMBER:

ARZL-0146

Draeger Safety Diagnostics, Inc.

BC



Calibration  
Certificate No. 1750.01

Calibration complies with ISO/IEC  
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-8483336

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by: VWR International, LLC, Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA 19087

Instrument Identification:

Model: 61220-601 S/N: 170297888 Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Temperature Calibration Bath TC-231	A79341		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5267	12/06/17	B6B30059
Temperature Calibration Bath TC-191	A42238		
Thermistor Module	A27129	12/01/17	1000401760
Temperature Probe	5202	12/19/17	B6B30058-1
Temperature Calibration Bath TC-218	A73332		
Thermistor Probe	5356	1/10/18	B7104024
Readout, Digital Thermometer	B5C344	3/12/18	B7314035
Temperature Calibration Bath TC-275	B16388		
Thermistor Probe	5357	1/06/18	B7104023
Readout, Digital Thermometer	B5C344	3/12/18	B7314035

Certificate Information:

Technician: 104 Procedure: CAL-06 Cal Date: 4/22/17 Due Date: 4/22/19  
Test Conditions: 23.9°C 61.0 %RH 1012 mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C		N.A.		0.002	-0.001	Y	-0.048	0.052	0.010	>4:1
°C		N.A.		25.000	24.999	Y	24.950	25.050	0.010	>4:1
°C		N.A.		49.998	50.000	Y	49.948	50.048	0.010	>4:1
°C		N.A.		99.998	100.003	Y	99.948	100.048	0.010	>4:1

This Instrument was calibrated using Instruments Traceable to National Institute of Standards and Technology.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement" (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min = As Left Nominal(Rounded) - Tolerance; Max = As Left Nominal(Rounded) + Tolerance; Date=MM/DD/YY

*Nicol Rodriguez*  
Nicol Rodriguez, Quality Manager

*Aaron Judice*  
Aaron Judice, Technical Manager

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometers change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598  
Phone 281 482-1714 Fax 281 482-9448 service@control3.com www.control3.com

Control Company is an ISO 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.  
Control Company is ISO 9001:2008 Quality Certified by (DNV) Det Norske Veritas, Certificate No. CERT-01805-2008-AQ-HOU-RvA.  
International Laboratory Accreditation Cooperation (ILAC) - Multilateral Recognition Arrangement (MRA).



**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ Other: \_\_\_\_\_

Serial Number:

DDWES3-0196

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ Other: \_\_\_\_\_

Serial Number:

DDWES3-0205

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ Other: \_\_\_\_\_

Serial Number:

DDRES3-0011

Certification Date:

9-26-17

Technician:

BC

Re-Certification Due Date:

9-26-18

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDUSP2-003

Certification Date:

9-8-17

Next Certification Due:

9-8-18

Probe Value:

98

Dräger, Inc.

BC



**Dräger**

**Simulator**

**CERTIFICATE OF ACCURACY**

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.  
(F.R. Vol. 59 No. 249 12/19/94 Notices)  
Draeger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ Other: \_\_\_\_\_

Serial Number:

DDAB-0014

Certification Date:

3-6-18

Technician:

BC

Re-Certification Due Date:

3-6-19

**Dräger**

**Alcotest 7110 Temperature Probe**

**CERTIFICATE OF ACCURACY**

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKP2-369

Certification Date:

3-6-18

Next Certification Due:

3-6-19

Probe Value:

99

Draeger, Inc.

BC



## State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

CHRIS CHRISTIE  
*Governor*

KIM GUADAGNO  
*Lt. Governor*

CHRISTOPHER S. PORRINO  
*Attorney General*

COLONEL JOSEPH R. FUENTES  
*Superintendent*

### **CERTIFICATION OF ANALYSIS 0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.


**ANALYSIS DATE:** 10/19/2016

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 16270


Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1203 to 0.1220 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 10, 2018.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
Ali M. Alaoui, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 20 day of October, 2016.

  
Notary  
**JOHN R LEAVER**  
ID # 2207138  
NOTARY PUBLIC  
STATE OF NEW JERSEY  
My Commission Expires Dec. 14, 2017



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable







## State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

CHRIS CHRISTIE  
*Governor*

KIM GUADAGNO  
*Lt. Governor*

CHRISTOPHER S. PORRINO  
*Attorney General*

COLONEL JOSEPH R. FUENTES  
*Superintendent*

### **CERTIFICATION OF ANALYSIS** **0.04 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.

**ANALYSIS DATE:** 08/29/2017

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 17240

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0483 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 10, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

Ali M. Alaouie, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 30<sup>th</sup> day of August, 2017.

Notary

**MARY ELIZABETH MCLAUGHLIN**

ID # 2052190

NOTARY PUBLIC

STATE OF NEW JERSEY

My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





## State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

CHRIS CHRISTIE  
*Governor*

KIM GUADAGNO  
*Lt. Governor*

CHRISTOPHER S. PORRINO  
*Attorney General*

COLONEL JOSEPH R. FUENTES  
*Superintendent*

### **CERTIFICATION OF ANALYSIS** **0.08 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.


**ANALYSIS DATE:** 09/07/2017

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 17250

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0963 to 0.0973 grams per 100 milliliters of solution.

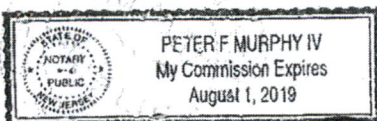
This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 15, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
Ali M. Alaouie, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 11 day of September, 2017.

  
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable







## State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

CHRIS CHRISTIE  
*Governor*

KIM GUADAGNO  
*Lt. Governor*

CHRISTOPHER S. PORRINO  
*Attorney General*

COLONEL JOSEPH R. FUENTES  
*Superintendent*

### **CERTIFICATION OF ANALYSIS** **0.16 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.


**ANALYSIS DATE:** 09/12/2017

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 17260

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1937 to 0.1957 grams per 100 milliliters of solution.

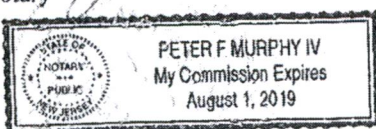
This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is August 21, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
Ali M. Alaoui, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 13 day of September, 2017.

  
Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable





## State of New Jersey

OFFICE OF THE ATTORNEY GENERAL  
DEPARTMENT OF LAW AND PUBLIC SAFETY  
DIVISION OF STATE POLICE  
POST OFFICE BOX 7068  
WEST TRENTON, NJ 08628-0068  
(609) 882-2000

PHILIP D. MURPHY  
Governor

SHEILA Y. OLIVER  
Lt. Governor

GURBIR S. GREWAL  
Attorney General

PATRICK J. CALLAHAN  
Colonel

### **CERTIFICATION OF ANALYSIS** **0.10 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

**ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION:** Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

**MANUFACTURER:** Draeger Safety, Inc.

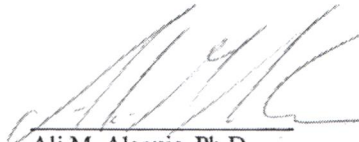
**ANALYSIS DATE:** 01/24/2018

**BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER:** 17420

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1230 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 11, 2019.

As Research Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.

  
Ali M. Alaouie, Ph.D.  
Research Scientist  
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 25<sup>th</sup> day of January, 2018.

Mary E. McLaughlin  
Notary

**MARY ELIZABETH MCLAUGHLIN**

ID # 2052190  
NOTARY PUBLIC  
STATE OF NEW JERSEY  
My Commission Expires Dec. 24, 2018



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer  
Printed on Recycled Paper and Recyclable






DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Bartłomiej P. Koziel**  
New Jersey State Police

IS AN ALIBI AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 102 OF  
THE LAWS OF 1986 IN THE OPERATION OF THE Aicotech 7110 NIKIII-C

A METHOD TO DETERMINE INTOXICATION  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 28th DAY OF July

TWO THOUSAND AND Eleven

  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

	DATE	Refresher Course PLACE	INSTRUCTOR
1.	7-15-13	M.I.P.A	R. J.
2.	9-16-15	BERGEN C.P.A	C. J.
3.	9-12-17	BERGEN C.P.A	C. J.
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 2036 (Rev. 03/10)

DEPARTMENT OF  
**Traffic and Public Safety**  
This is to certify that

**Bartłomiej Koziel**  
**Breath Test Coordinator/Instructor**

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1966 IN THE OPERATION OF THE **Alcotest 7110 MKIII-C**

A METHOD TO DETERMINE INTOXICATION.  
GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS **16th** DAY OF **December**

TWO THOUSAND AND **Sixteen**

*[Signature]*  
SUPERINTENDENT  
NEW JERSEY STATE POLICE

*[Signature]*  
ATTORNEY GENERAL  
STATE OF NEW JERSEY

ORIGINAL COURSE DATES:

	DATE	Refresher Course PLACE	INSTRUCTOR
1.			
2.			
3.			
4.			
5.			
6.			
7.			
8.			
9.			

S.P. 2998 (Rev. 07/16)





# Dräger



## Alcotest 7110 Temperature Probe

### CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKP2 - 369

Certification Date:

3-6-18

Next Certification Due:

3-6-19

Probe Value:

99

Draeger, Inc.

BC





# Dräger

## Simulator

### CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.

(F.R. Vol. 59 No. 249 12/19/94 Notices)

Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ Other: \_\_\_\_\_

Serial Number:

DDAB-0014

Certification Date:

3-6-18

Technician:

BC

Re-Certification Due Date:

3-6-19

