

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)

Draeger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDAB - 0014

Certification Date:

12.31.20

Technician:

AM

Re-Certification Due Date:

12.31.21



Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.

For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXK P2-369

Certification Date:

12-31-20

Next Certification Due:

12-31-21

Probe Value:

102

Draeger, Inc.


an

Alcotest 7110 Calibration Record

Equipment

Location:	Alcotest 7110 MKIII-C	Serial No.:	ARXA-0037
Calibration File No.:	WALL TOWNSHIP POLICE		
Certification File No.:	02072	Calib. Date:	04/15/2021
Linearity File No.:	02065	Cert. Date:	10/27/2020
Solution File No.:	02066	Lin. Date:	10/27/2020
Sequential File No.:	02071	Soln. Date:	12/10/2020
	02072	File Date:	04/15/2021
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDAB-0014
Solution Control Lot:	19270	Expires:	10/14/2021
		Bottle No.:	0626

Coordinator

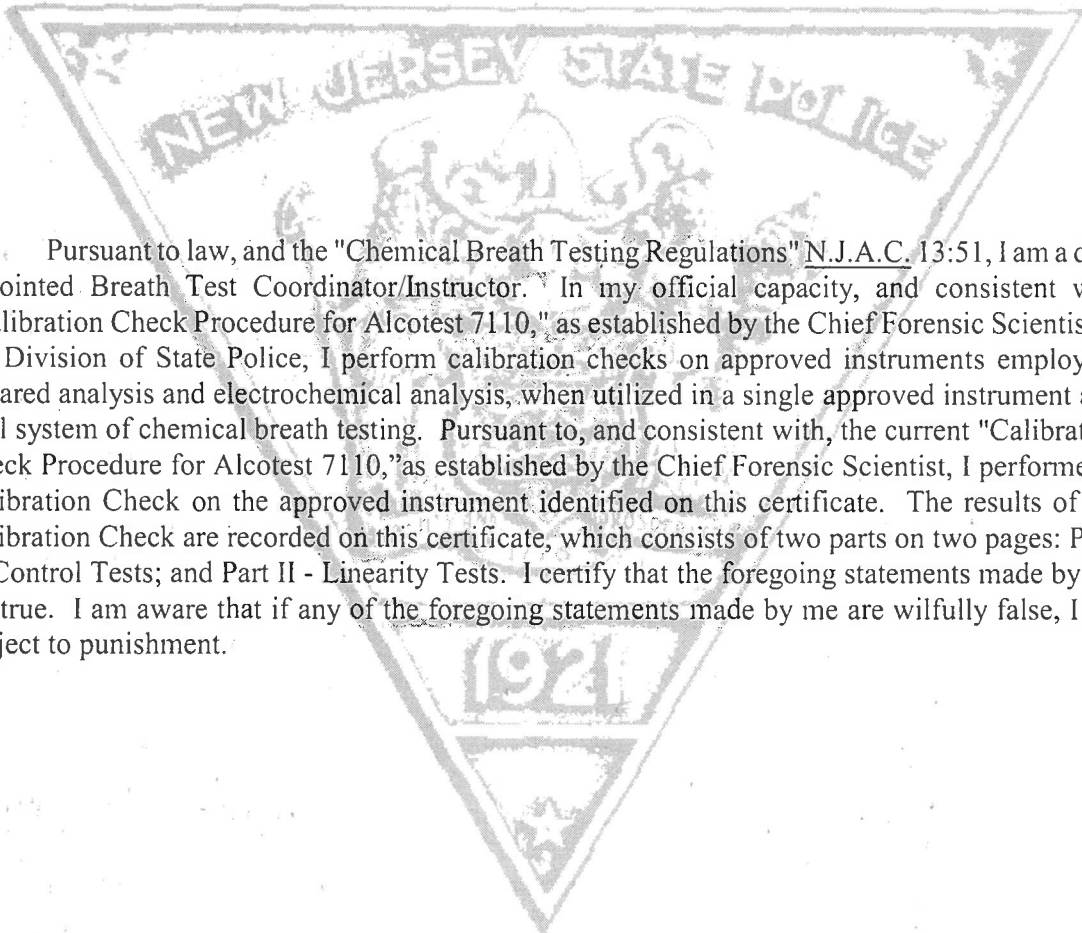
Last Name:	LUTZ	First Name:	DENNIS	MI:	J
Signature:				Badge No.:	7045
				Date:	04/15/2021

*Black Key Temperature Probe Serial.....#

DOEEP2-060 (DL)

*Digital NIST Temperature Measuring System Serial.....#

200 357 843 (DL)



Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part I - Control Tests

Equipment

Alcotest 7110 MKIII-C
Location: WALL TOWNSHIP POLICE
Serial No.: ARXA-0037
Calibration File No.: 02072 Calib. Date: 04/15/2021 Calib. No.: 00043
Certification File No.: 02073 Cert. Date: 04/15/2021 Cert. No.: 00033
Linearity File No.: 02066 Lin. Date: 10/27/2020 Lin. No.: 00032
Solution File No.: 02071 Soln. Date: 12/10/2020 Soln. No.: 00419
Sequential File No.: 02073 File Date: 04/15/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0014
Control Solution %: 0.100% Expires: 10/14/2021
Solution Control Lot: 19270 Bottle No.: 0626

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:30D		
Control 1 EC	0.099%	11:30D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	11:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:31D		
Control 2 EC	0.099%	11:31D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.099%	11:31D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:32D		
Control 3 EC	0.099%	11:33D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	11:33D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:33D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: Tpr I Lutz 7045

Badge No.: 7045

Date: 04/15/2021

Pursuant to law, and the "Chemical Breath Testing Regulations" N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity, and consistent with "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on approved instruments employing infrared analysis and electrochemical analysis, when utilized in a single approved instrument as a dual system of chemical breath testing. Pursuant to, and consistent with, the current "Calibration Check Procedure for Alcotest 7110," as established by the Chief Forensic Scientist, I performed a Calibration Check on the approved instrument identified on this certificate. The results of my Calibration Check are recorded on this certificate, which consists of two parts on two pages: Part I - Control Tests; and Part II - Linearity Tests. I certify that the foregoing statements made by me are true. I am aware that if any of the foregoing statements made by me are wilfully false, I am subject to punishment.

Alcotest 7110 Calibration Certificate

Part II - Linearity Tests

Equipment

Location: Alcotest 7110 MKIII-C
WALL TOWNSHIP POLICE

Calibration File No.: 02072

Calib. Date: 04/15/2021

Certification File No.: 02073

Cert. Date: 04/15/2021

Linearity File No.: 02074

Lin. Date: 04/15/2021

Solution File No.: 02071

Soln. Date: 12/10/2020

Sequential File No.: 02074

File Date: 04/15/2021

Serial No.: ARXA-0037

Calib. No.: 00043

Cert. No.: 00033

Lin. No.: 00033

Soln. No.: 00419

Calibrating Unit: WET

Model No.: CU-34

Serial No.: DDSC S3-0001

Control Solution %: 0.040%

Expires: 11/04/2021

Solution Control Lot: 19310

Bottle No.: 0329

Calibrating Unit: WET

Model No.: CU-34

Serial No.: DDXC S3-0020

Control Solution %: 0.080%

Expires: 11/11/2021

Solution Control Lot: 19320

Bottle No.: 0809

Calibrating Unit: WET

Model No.: CU-34

Serial No.: DDMK S3-0006

Control Solution %: 0.160%

Expires: 12/02/2021

Solution Control Lot: 19360

Bottle No.: 0850

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	11:48D		
Control 1 EC	0.041%	11:48D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.040%	11:48D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:50D		
Control 2 EC	0.041%	11:50D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.039%	11:50D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:52D		
Control 3 EC	0.081%	11:52D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.078%	11:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:54D		
Control 4 EC	0.079%	11:55D	34.0°C	*** TEST PASSED ***
Control 4 IR	0.078%	11:55D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:56D		
Control 5 EC	0.158%	11:57D	34.0°C	*** TEST PASSED ***
Control 5 IR	0.157%	11:57D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	11:58D		
Control 6 EC	0.158%	11:59D	34.0°C	*** TEST PASSED ***
Control 6 IR	0.157%	11:59D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	12:00D		

All tests within acceptable tolerance.

Coordinator

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: Tpr I Dent 7045

Badge No.: 7045

Date: 04/15/2021

Calibrating Unit New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: WALL TOWNSHIP POLICE
Serial No.: ARXA-0037
Calibration File No.: 02072 Calib. Date: 04/15/2021 Calib. No.: 00043
Certification File No.: 02073 Cert. Date: 04/15/2021 Cert. No.: 00033
Linearity File No.: 02074 Lin. Date: 04/15/2021 Lin. No.: 00033
Solution File No.: 02075 Soln. Date: 04/15/2021 Soln. No.: 00420
Sequential File No.: 02075 File Date: 04/15/2021

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0014
Control Solution %: 0.100% Expires: 06/10/2021
Solution Control Lot: 19150 Bottle No.: 1193

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	13:16D		
Control 1 EC	0.099%	13:16D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	13:16D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:17D		
Control 2 EC	0.097%	13:18D	34.1°C	*** TEST PASSED ***
Control 2 IR	0.098%	13:18D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:18D		
Control 3 EC	0.097%	13:19D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.097%	13:19D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	13:20D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with
Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Temperature Probe Serial Number: DDXKP2-369 (D)

Changed By:

Last Name: LUTZ

First Name: DENNIS

MI: J

Signature: Tpr I Dent 7045

Badge No.: 7045

Date: 04/15/2021

**Alcotest 7110 MKIII-C Calibration
NIST-Traceable Digital Thermometer Readings**

Coordinator:

Tpr I Dennis J Lotz
Name

7045
Badge No.

Location:

Wall Township Police
Agency

ARXA-0037
Alcotest Serial No.

Equipment:

200 357 843
Digital NIST Temperature Measuring System Serial No.

Simulator Solution Concentration	CU-34 Simulator Serial No.	Time Simulators Started to Heat	Time Temp. Reading Obtained	Temp. Reading on NIST Traceable Thermometer
0.04%	DDSL 53-0001	09:58 D	11:16 D	33.9°C
0.08%	DDXL 53-0020	09:58 D	11:17 D	33.9°C
0.10%	DDAB-0014	09:58 D	11:18 D	34.0°C
0.16%	DDMK 53-0006	09:58 D	11:20 D	33.9°C

Pursuant to law and the "Chemical Breath Testing Regulations" established at N.J.A.C. 13:51, I am a duly appointed Breath Test Coordinator/Instructor. In my official capacity and consistent with the "Calibration Check Procedure for Alcotest 7110" as established by the Chief Forensic Scientist of the Division of State Police, I perform calibration checks on Alcotest 7110 MKIII-C instruments. Pursuant to and consistent with the current "Calibration Check Procedure for Alcotest 7110", I performed a Calibration Check Procedure on the Alcotest 7110 MKIII-C instrument identified on this certificate. Pursuant to the current "Calibration Check Procedure for Alcotest 7110", I used the Digital NIST-traceable Temperature Measuring System identified on this certificate to confirm that the temperatures of the 0.10%, 0.04%, 0.08%, and 0.16% Simulator Solutions used in the respective CU-34 Simulators identified on this certificate, were 34.0 degrees Celsius \pm 0.2 degrees Celsius. I hereby certify that I truthfully recorded on this certificate the temperatures of each of the simulator solutions as shown on the Digital NIST-traceable Temperature Measuring System thermometer. I am aware that if any of the foregoing statements made by me are willfully false, I am subject to punishment.

Tpr I [Signature] 7045
Coordinator's Signature

4-15-21
Date

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDSC33-0001

Certification Date:

6.2.20

Technician:

MB

Re-Certification Due Date:

6.2.21

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDXCS3-0020

Certification Date:

6.2.20

Technician:

MB

Re-Certification Due Date:

6.2.21

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Draeger, Inc.

- ☒ Model: ALCOTEST CU34
☐ Model: MARK IIA
☐ X-Cal 2000 (Alcosim)
☐ Other: _____

Serial Number:

DDMK53-0004

Certification Date:

10-15-20

Technician:

MB

Re-Certification Due Date:

10-15-21

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications.
For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDEEP2-060

Certification Date:

6-3-20

Next Certification Due:

6-3-21

Probe Value:

106

Draeger, Inc.

MB



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11349797

Traceable® Certificate of Calibration for Digital Thermometer

Manufactured for and distributed by : VWR International LLC Radnor Corporate Center, Bldg 1, Ste 200, 100 Matsonford Road, Radnor, PA, 19087

Instrument Identification:

Model: 61220-601,

S/N: 200357843

Manufacturer: Control Company

Standards/Equipment:

Description	Serial Number	Due Date	NIST Traceable Reference
Thermistor Module	A27129	04 Feb 2021	1000451212
Temperature Calibration Bath	A42238		
Temperature Calibration Bath	B01375		
Temperature Probe	5394	21 Feb 2021	C0220030
Temperature Calibration Bath	B16388		
Temperature Probe	5267	21 Feb 2021	C0220028
Temperature Calibration Bath	B3A444		
Thermistor Module	B96381	16 Jul 2020	B9626028
Temperature Probe	5398	16 Jul 2020	B9605083
Thermistor Module	B96382	19 Aug 2020	B9628006
Temperature Probe	5410	13 Sep 2020	B9801031

Certificate Information:

Technician: 420

Procedure: CAL-06

Cal Date: 15 Jun 2020

Cal Due Date: 15 Jun 2022

Test Conditions: 52.44%RH 23.46°C 1018mBar

Calibration Data: (New Instrument)

Unit(s)	Nominal	As Found	In Tol	Nominal	As Left	In Tol	Min	Max	±U	TUR
°C	N.A.	N.A.		0.000	0.001	Y	-0.05	0.05	0.0087	>4:1
°C	N.A.	N.A.		25.001	25.001	Y	24.951	25.051	0.0087	>4:1
°C	N.A.	N.A.		50.002	50.001	Y	49.952	50.052	0.0087	>4:1
°C	N.A.	N.A.		100.001	99.998	Y	99.951	100.051	0.0087	>4:1

This certificate indicates Traceability to standards provided by (NIST) National Institute of Standards and Technology and/or a National Standards Laboratory.

A Test Uncertainty Ratio of at least 4:1 is maintained unless otherwise stated and is calculated using the expanded measurement uncertainty. Uncertainty evaluation includes the instrument under test and is calculated in accordance with the ISO "Guide to the Expression of Uncertainty in Measurement": (GUM). The uncertainty represents an expanded uncertainty using a coverage factor k=2 to approximate a 95% confidence level. In tolerance conditions are based on test results falling within specified limits with no reduction by the uncertainty of the measurement. The results contained herein relate only to the item calibrated. This certificate shall not be reproduced except in full, without written approval of Control Company.

Nominal=Standard's Reading; As Left=Instrument's Reading; In Tol=In Tolerance; Min/Max=Acceptance Range; ±U=Expanded Measurement Uncertainty; TUR=Test Uncertainty Ratio; Accuracy=±(Max-Min)/2; Min=As Left Nominal(Rounded) - Tolerance; Max= As Left Nominal(Rounded) + Tolerance;

Nicol Rodriguez

Nicol Rodriguez, Quality Manager

Marisa Elms

Marisa Elms, Technical Manager

Note :

Maintaining Accuracy:

In our opinion once calibrated your Digital Thermometer should maintain its accuracy. There is no exact way to determine how long calibration will be maintained. Digital Thermometer change little, if any at all, but can be affected by aging, temperature, shock, and contamination.

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



Calibration complies with ISO/IEC
17025, ANSI/NCSL Z540-1, and 9001



Cert. No.: 4000-11349797

Traceable® Certificate of Calibration for Digital Thermometer

Recalibration:

For factory calibration and re-certification traceable to National Institute of Standards and Technology contact Control Company.

Issue Date : 15 Jun 2020

CONTROL COMPANY 12554 Galveston RD Suite B230 Webster TX USA 77598
Phone 281 482-1714 Fax 281 482-9448 sales@control3.com www.traceable.com

Control Company is an ISO/IEC 17025:2005 Calibration Laboratory Accredited by (A2LA) American Association for Laboratory Accreditation, Certificate No. 1750.01.
Control Company is ISO 9001:2015 Quality Certified by DNV GL, Certificate No. CERT-01805-2006-AQ-HOU-ANAB.
International Laboratory Accreditation Cooperation - Multilateral Recognition Arrangement (ILAC-MRA).



State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS 0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 10/21/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19270

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1216 to 0.1232 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is October 14, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 28 day of October, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024

"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.040 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0469 to 0.0499 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 11/14/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19310

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0485 to 0.0489 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 04, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 15 day of November, 2019.

Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.080 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.0939 to 0.0997 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 11/20/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19320

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.0971 to 0.0985 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is November 11, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 21 day of November, 2019.


Notary

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

*New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable*





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.160 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1878 to 0.1994 grams per 100 milliliters of solution.

MANUFACTURER: Draeger, Inc.


ANALYSIS DATE: 12/11/2019

BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19360

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1936 to 0.1956 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is December 02, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences

Sworn to and subscribed before me this 18 day of December, 2019.

Notary 

KAREN E. STAHL
NOTARY PUBLIC OF NEW JERSEY
Commission # 50110522
My Commission Expires 8/13/2024



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable





State of New Jersey

OFFICE OF THE ATTORNEY GENERAL
DEPARTMENT OF LAW AND PUBLIC SAFETY
DIVISION OF STATE POLICE
POST OFFICE BOX 7068
WEST TRENTON, NJ 08628-0068
(609) 882-2000

PHILIP D. MURPHY
Governor

SHEILA Y. OLIVER
Lt. Governor

GURBIR S. GREWAL
Attorney General

PATRICK J. CALLAHAN
Colonel

CERTIFICATION OF ANALYSIS **0.100 PERCENT BREATH ALCOHOL SIMULATOR SOLUTION**

ACCEPTANCE SPECIFICATIONS FOR BREATH ALCOHOL SIMULATOR SOLUTION: Ethyl alcohol concentration within, but not exceeding, the range of 0.1174 to 0.1246 grams per 100 milliliters of solution.

MANUFACTURER: Draeger Safety, Inc.


ANALYSIS DATE: 06/20/2019

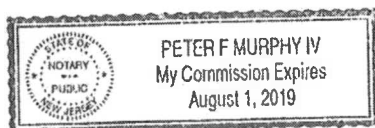
BREATH ALCOHOL SIMULATOR SOLUTION LOT NUMBER: 19150

Representative samples of the above-referenced Lot Number were tested by Gas Chromatography and found to have a mean ethyl alcohol concentration range of 0.1196 to 0.1212 grams per 100 milliliters of solution.

This lot of breath alcohol simulator solution may be utilized as a known traceable standard for the purpose of conducting periodic tests, pursuant to N.J.A.C. 13:51-4.3, of approved breath test instruments (N.J.A.C. 13:51-3.5) utilized by law enforcement agencies in this State. The manufacturer's expiration date for this lot of breath alcohol simulator solution is June 10, 2021.

As Assistant Chief Forensic Scientist for the Division of State Police, I hereby certify and attest that the tests and results documented in this Certificate of Analysis were performed at the Office of Forensic Sciences of the Division of State Police on properly functioning and calibrated instruments and equipment. All procedures utilized are accurate, objective, and performed on a routine basis by personnel within the Office of Forensic Sciences, in accordance with their professional duties and responsibilities.


Michael Kennedy
Assistant Chief Forensic Scientist
NJSP Office of Forensic Sciences



Sworn to and subscribed before me this 26th day of June, 2019.


Notary



"An Internationally Accredited Agency"

New Jersey Is An Equal Opportunity Employer
Printed on Recycled Paper and Recyclable



DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Dennis J. Lutz

Breath Test Coordinator/Instructor

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1946 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 29th DAY OF January

TWO THOUSAND AND Nineteen

[Signature]
COLONEL
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. _____	_____	_____
2. _____	_____	_____
3. _____	_____	_____
4. _____	_____	_____
5. _____	_____	_____
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2538 (Rev. 01/18)

DEPARTMENT OF
Traffic and Public Safety
This is to certify that

Dennis J. Lutz
New Jersey State Police

IS QUALIFIED AND COMPETENT TO CONDUCT CHEMICAL BREATH ANALYSES PURSUANT TO CHAPTER 142 OF

THE LAWS OF 1946 IN THE OPERATION OF THE Alcotest 7110 MKIII-C

A METHOD TO DETERMINE INTOXICATION

GIVEN UNDER MY HAND AT TRENTON, NEW JERSEY THIS 1st DAY OF October

TWO THOUSAND AND Nine

[Signature]
COLONEL
NEW JERSEY STATE POLICE

[Signature]
ATTORNEY GENERAL
STATE OF NEW JERSEY

ORIGINAL COURSE DATES

DATE	Refresher Course PLACE	INSTRUCTOR
1. <u>2-3-11</u>	<u>OCPA</u>	<u>Wm. Horn</u>
2. <u>1/24/13</u>	<u>OCPA</u>	<u>Adam Stankovic</u>
3. <u>11-23-15</u>	<u>GCPA</u>	<u>M. Gonzalez</u>
4. <u>4/6/17</u>	<u>LAKELAND</u>	<u>Adam Stankovic</u>
5. <u>8/22/19</u>	<u>NJSP Gateway</u>	<u>[Signature]</u>
6. _____	_____	_____
7. _____	_____	_____
8. _____	_____	_____
9. _____	_____	_____

S.P. 2538 (Rev. 07/17)



Dräger

Alcotest 7110

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 has been tested for accuracy and found to be in compliance with the National Highway Traffic Safety Administration Standard for evidential breath testing devices. The Alcotest MKIII-C is compliant as a "mobile" and "nonmobile" EBT with 49 FR 48854, 49 FR 48884, and 58 FR 48705. The manufacturer recommends accuracy verification of this instrument within 12 months of the calibration date below, or sooner, according to your state's specifications.

Certification Date:

Serial Number:

2-6-2020

ARXA-0037

Draeger, Inc.

BS

Dräger

Simulator

CERTIFICATE OF ACCURACY

This Certificate of Accuracy verifies that the specified unit has been examined and found to be in compliance with National Highway and Traffic Safety Administration regulations for devices used to calibrate Evidential Breath Testers.
(F.R. Vol. 59 No. 249 12/19/94 Notices)
Dräger, Inc.

☒ Model: ALCOTEST CU34

☐ Model: MARK IIA

☐ X-Cal 2000 (Alcosim)

☐ Other: _____

Serial Number:

DDAB-0014

Certification Date:

12.31.20

Technician:

am

Re-Certification Due Date:

12.31.21

Dräger

Alcotest 7110 Temperature Probe

CERTIFICATE OF ACCURACY

This is to certify that the Alcotest 7110 Temperature Probe has been tested for accuracy with instrumentation that is traceable to the National Institute of Standards and Technology (NIST). The manufacturer recommends accuracy verification of the Temperature Probe within 12 months of the certification date below, or sooner, according to your state's specifications. For accurate temperature readings, the probe value on this certificate, noted below, must be programmed into the Alcotest 7110.

Serial Number Temp Probe:

DDXKP2-369

Certification Date:

12.31.20

Next Certification Due:

12.31.21

Probe Value:

102

Dräger, Inc.

am