

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0037
Location: WALL TOWNSHIP POLICE
Calibration File No.: 01363 Calib. Date: 09/08/2015 Calib. No.: 00026
Certification File No.: 01364 Cert. Date: 09/08/2015 Cert. No.: 00018
Linearity File No.: 01365 Lin. Date: 09/08/2015 Lin. No.: 00018
Solution File No.: 01373 Soln. Date: 10/09/2015 Soln. No.: 00225
Sequential File No.: 01373 File Date: 10/09/2015

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0014
Control Solution %: 0.100% Expires: 06/13/2017
Solution Control Lot: 15F139 Bottle No.: 0489

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:50D		
Control 1 EC	0.098%	09:51D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.096%	09:51D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:51D		
Control 2 EC	0.097%	09:52D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	09:52D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:52D		
Control 3 EC	0.097%	09:53D	34.1°C	*** TEST PASSED ***
Control 3 IR	0.097%	09:53D	34.1°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:54D		

All tests within acceptable tolerance.

On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.


Changed By:

Last Name: KAZANOWSKY

First Name: PTL.

MI: A

Signature: _____

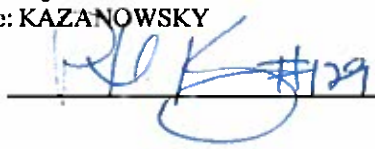

Badge No.: 129

Date: 10/09/2015