

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARZL-0146
Location: WALL TOWNSHIP POLICE
Calibration File No.: 01337 **Calib. Date:** 07/21/2017 **Calib. No.:** 00027
Certification File No.: 01338 **Cert. Date:** 07/21/2017 **Cert. No.:** 00023
Linearity File No.: 01339 **Lin. Date:** 07/21/2017 **Lin. No.:** 00023
Solution File No.: 01402 **Soln. Date:** 12/24/2017 **Soln. No.:** 00259
Sequential File No.: 01402 **File Date:** 12/24/2017

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDAB-0015
Control Solution %: 0.100% **Expires:** 09/14/2019
Solution Control Lot: 17290 **Bottle No.:** 0099

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	22:39S		
Control 1 EC	0.099%	22:40S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	22:40S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:40S		
Control 2 EC	0.097%	22:41S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.098%	22:41S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:42S		
Control 3 EC	0.097%	22:42S	33.9°C	*** TEST PASSED ***
Control 3 IR	0.097%	22:42S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	22:43S		

All tests within acceptable tolerance.

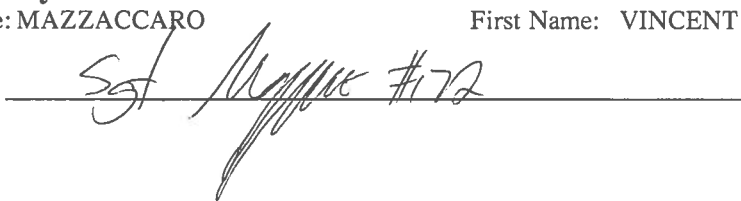
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: MAZZACCARO

First Name: VINCENT

MI: J

Signature: 

Badge No.: 172

Date: 12/24/2017