

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: WALL TOWNSHIP POLICE
Serial No.: ARXA-0037
Calibration File No.: 01858 Calib. Date: 11/16/2018 Calib. No.: 00036
Certification File No.: 01859 Cert. Date: 11/16/2018 Cert. No.: 00027
Linearity File No.: 01860 Lin. Date: 11/16/2018 Lin. No.: 00027
Solution File No.: 01863 Soln. Date: 12/14/2018 Soln. No.: 00336
Sequential File No.: 01863 File Date: 12/14/2018

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDXB S3-114
Control Solution %: 0.100% Expires: 05/10/2020
Solution Control Lot: 18150 Bottle No.: 0680

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:15S		
Control 1 EC	0.100%	09:15S	33.9°C	*** TEST PASSED ***
Control 1 IR	0.100%	09:15S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16S		
Control 2 EC	0.099%	09:17S	33.9°C	*** TEST PASSED ***
Control 2 IR	0.100%	09:17S	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:18S		
Control 3 EC	0.097%	09:18S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:18S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:19S		

All tests within acceptable tolerance.

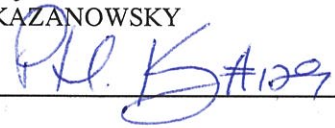
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KAZANOWSKY

First Name: PTL

MI: A

Signature: 

Badge No.: 129

Date: 12/14/2018