

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARZL-0146
Location: WALL TOWNSHIP POLICE
Calibration File No.: 01601 Calib. Date: 04/17/2019 Calib. No.: 00031
Certification File No.: 01602 Cert. Date: 04/17/2019 Cert. No.: 00027
Linearity File No.: 01603 Lin. Date: 04/17/2019 Lin. No.: 00027
Solution File No.: 01623 Soln. Date: 05/23/2019 Soln. No.: 00303
Sequential File No.: 01623 File Date: 05/23/2019

Calibrating Unit: WET Model No.: CU-34 Serial No.: DDAB-0014
Control Solution %: 0.100% Expires: 01/08/2021
Solution Control Lot: 19020 Bottle No.: 1020

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:12D		
Control 1 EC	0.098%	09:13D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	09:13D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:14D		
Control 2 EC	0.097%	09:14D	33.9°C	*** TEST PASSED ***
Control 2 IR	0.099%	09:14D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:15D		
Control 3 EC	0.097%	09:16D	33.9°C	*** TEST PASSED ***
Control 3 IR	0.100%	09:16D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	09:16D		

All tests within acceptable tolerance.

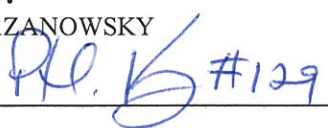
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: KAZANOWSKY

First Name: PTL

MI: A

Signature:  #129

Badge No.: 129

Date: 05/23/2019