

Calibrating Unit New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARXA-0037
Location: WALL TOWNSHIP POLICE
Calibration File No.: 01983 **Calib. Date:** 09/03/2019 **Calib. No.:** 00038
Certification File No.: 01984 **Cert. Date:** 09/03/2019 **Cert. No.:** 00029
Linearity File No.: 01985 **Lin. Date:** 09/03/2019 **Lin. No.:** 00029
Solution File No.: 01991 **Soln. Date:** 09/21/2019 **Soln. No.:** 00383
Sequential File No.: 01991 **File Date:** 09/21/2019

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDXB S3-114
Control Solution %: 0.100% **Expires:** 06/10/2021
Solution Control Lot: 19150 **Bottle No.:** 1289

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:42D		
Control 1 EC	0.099%	18:43D	33.9°C	*** TEST PASSED ***
Control 1 IR	0.098%	18:43D	33.9°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:43D		
Control 2 EC	0.094%	18:44D	33.9°C	CONTROL TEST FAILED
Control 2 IR	0.098%	18:44D	33.9°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	18:45D		
Control 3 EC	0.094%	18:45D	33.9°C	CONTROL TEST FAILED
Control 3 IR	0.098%	18:45D	33.9°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	18:46D		

Test results are not within acceptable range.

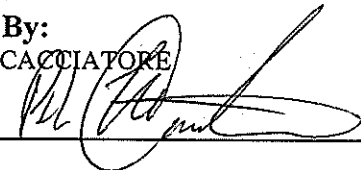
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CACCIATORE

First Name: MICHAEL

MI: J

Signature:  #187

Badge No.: 187

Date: 09/21/2019