

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARZL-0146
Location: WALL TOWNSHIP POLICE
Calibration File No.: 01731 **Calib. Date:** 09/03/2019 **Calib. No.:** 00032
Certification File No.: 01732 **Cert. Date:** 09/03/2019 **Cert. No.:** 00028
Linearity File No.: 01733 **Lin. Date:** 09/03/2019 **Lin. No.:** 00028
Solution File No.: 01743 **Soln. Date:** 09/21/2019 **Soln. No.:** 00321
Sequential File No.: 01743 **File Date:** 09/21/2019

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDXB S3-113
Control Solution %: 0.100% **Expires:** 06/10/2021
Solution Control Lot: 19150 **Bottle No.:** 0874

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	18:28D		
Control 1 EC	0.097%	18:29D	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	18:29D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:30D		
Control 2 EC	0.097%	18:30D	34.0°C	*** TEST PASSED ***
Control 2 IR	0.097%	18:30D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:31D		
Control 3 EC	0.096%	18:32D	34.0°C	*** TEST PASSED ***
Control 3 IR	0.097%	18:32D	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	18:33D		

All tests within acceptable tolerance.

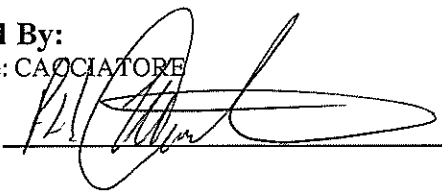
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CAOCIA TORE

First Name: MICHAEL

MI: J

Signature: 

Badge No.: 187

Date: 09/21/2019