

Calibrating Unit

New Standard Solution Report

Equipment Alcotest 7110 MKIII-C Serial No.: ARZL-0146
Location: WALL TOWNSHIP POLICE
Calibration File No.: 01932 **Calib. Date:** 04/15/2021 **Calib. No.:** 00037
Certification File No.: 01933 **Cert. Date:** 04/15/2021 **Cert. No.:** 00032
Linearity File No.: 01934 **Lin. Date:** 04/15/2021 **Lin. No.:** 00032
Solution File No.: 01984 **Soln. Date:** 07/17/2021 **Soln. No.:** 00367
Sequential File No.: 01984 **File Date:** 07/17/2021

Calibrating Unit: WET **Model No.:** CU-34 **Serial No.:** DDAB-0015
Control Solution %: 0.100% **Expires:** 03/30/2022
Solution Control Lot: 20180 **Bottle No.:** 0636

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	09:01D		
Control 1 EC	0.000%	09:01D	34.0°C	CONTROL TEST FAILED
Control 1 IR	0.000%	09:01D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	09:01D		
Control 2 EC	0.000%	09:02D	34.0°C	CONTROL TEST FAILED
Control 2 IR	0.000%	09:02D	34.0°C	CONTROL TEST FAILED
Ambient Air Blank	0.000%	09:03D		
Control 3 EC	-.---%	09:03D	34.0°C	CTRL GAS SUPPLY
Control 3 IR	-.---%	09:03D	34.0°C	CTRL GAS SUPPLY
Ambient Air Blank	-.---%	--:--		

Test results are not within acceptable range.

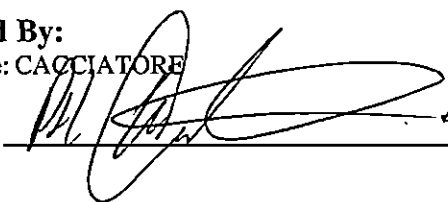
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CACCIATORE

First Name: MICHAEL

MI: J

Signature: 

Badge No.: 187

Date: 07/17/2021