

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: WALL TOWNSHIP POLICE
Serial No.: ARXA-0037
Calibration File No.: 02086
Calib. Date: 10/13/2021
Calib. No.: 00044
Certification File No.: 02087
Cert. Date: 10/13/2021
Cert. No.: 00034
Linearity File No.: 02088
Lin. Date: 10/13/2021
Lin. No.: 00034
Solution File No.: 02091
Soln. Date: 11/07/2021
Soln. No.: 00428
Sequential File No.: 02091
File Date: 11/07/2021

Calibrating Unit: WET
Control Solution %: 0.100%
Solution Control Lot: 20460
Model No.: CU-34
Serial No.: DDXB.S3-113
Expires: 10/21/2022
Bottle No.: 1391

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	04:40S		
Control 1 EC	0.096%	04:41S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.099%	04:41S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:41S		
Control 2 EC	0.095%	04:42S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.098%	04:42S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:43S		
Control 3 EC	0.096%	04:43S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	04:43S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	04:44S		

All tests within acceptable tolerance.

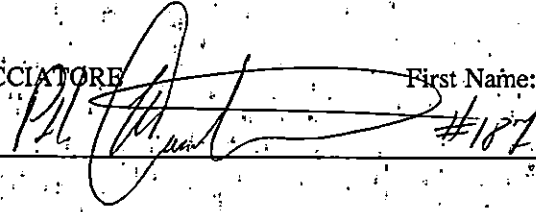
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CACCIATORE

First Name: MICHAEL

MI: J

Signature: 

Badge No.: 187

Date: 11/07/2021