

Calibrating Unit

New Standard Solution Report

Equipment	Alcotest 7110 MKIII-C	Serial No.:	ARZL-0146
Location:	WALL TOWNSHIP POLICE		
Calibration File No.:	02021	Calib. Date:	10/13/2021
Certification File No.:	02022	Calib. No.:	00038
Linearity File No.:	02023	Cert. Date:	10/13/2021
Solution File No.:	02034	Cert. No.:	00033
Sequential File No.:	02034	Lin. Date:	10/13/2021
		Lin. No.:	00033
		Soln. Date:	11/19/2021
		Soln. No.:	00375
		File Date:	11/19/2021
Calibrating Unit:	WET	Model No.:	CU-34
Control Solution %:	0.100%	Serial No.:	DDXB S3-114
Solution Control Lot:	20180	Expires:	03/30/2022
		Bottle No.:	0843

Function	Result %BAC	Time HH:MM	Temperature Simulator (°C)	Comment(s) or Error(s)
Ambient Air Blank	0.000%	10:34S		
Control 1 EC	0.101%	10:34S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.101%	10:34S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:35S		
Control 2 EC	0.100%	10:36S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.101%	10:36S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:36S		
Control 3 EC	0.100%	10:37S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.100%	10:37S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	10:38S		

All tests within acceptable tolerance.

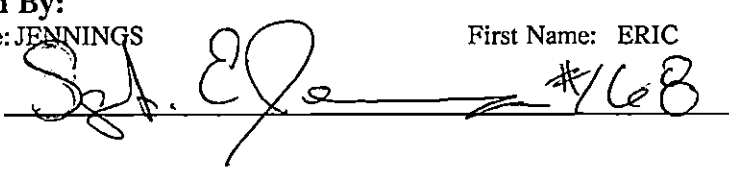
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: JENNINGS

First Name: ERIC

MI: R

Signature: 

Badge No.: 168

Date: 11/19/2021