

Calibrating Unit

New Standard Solution Report

Equipment

Alcotest 7110 MKIII-C
Location: WALL TOWNSHIP POLICE
Serial No.: ARXA-0037
Calibration File No.: 02086
Calib. Date: 10/13/2021
Calib. No.: 00044
Certification File No.: 02087
Cert. Date: 10/13/2021
Cert. No.: 00034
Linearity File No.: 02088
Lin. Date: 10/13/2021
Lin. No.: 00034
Solution File No.: 02101
Soln. Date: 01/21/2022
Soln. No.: 00434
Sequential File No.: 02101
File Date: 01/21/2022
Calibrating Unit: WET
Model No.: CU-34
Serial No.: DDXB S3-113
Control Solution %: 0.100%
Expires: 10/21/2022
Solution Control Lot: 20460
Bottle No.: 1447

Function	Result	Time	Temperature	Comment(s)
	%BAC	HH:MM	Simulator (°C)	or Error(s)
Ambient Air Blank	0.000%	07:19S		
Control 1 EC	0.097%	07:20S	34.0°C	*** TEST PASSED ***
Control 1 IR	0.098%	07:20S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:20S		
Control 2 EC	0.096%	07:21S	34.0°C	*** TEST PASSED ***
Control 2 IR	0.099%	07:21S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:22S		
Control 3 EC	0.097%	07:22S	34.0°C	*** TEST PASSED ***
Control 3 IR	0.099%	07:22S	34.0°C	*** TEST PASSED ***
Ambient Air Blank	0.000%	07:23S		

All tests within acceptable tolerance.

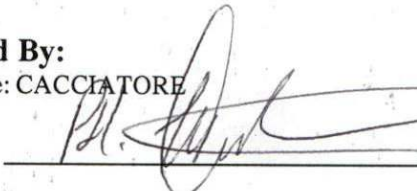
On this date, I installed the above indicated "NEW SOLUTION" in accordance with Alcotest 7110 operator training and procedures established by the (NJSP) Chief Forensic Scientist.

Changed By:

Last Name: CACCIATORE

First Name: MICHAEL

MI: J

Signature: 

Badge No.: 187

Date: 01/21/2022